Principles of MRI

EE225E / BIO265

Instructor: Miki Lustig
UC Berkeley, EECS

Today....

- Administration
  - http://www-inst.eecs.berkeley.edu/~ee225e/sp12/

- Intro to Medical Imaging and MRI

Medical Imaging (Before 1895)

- Only way to see is to cut!

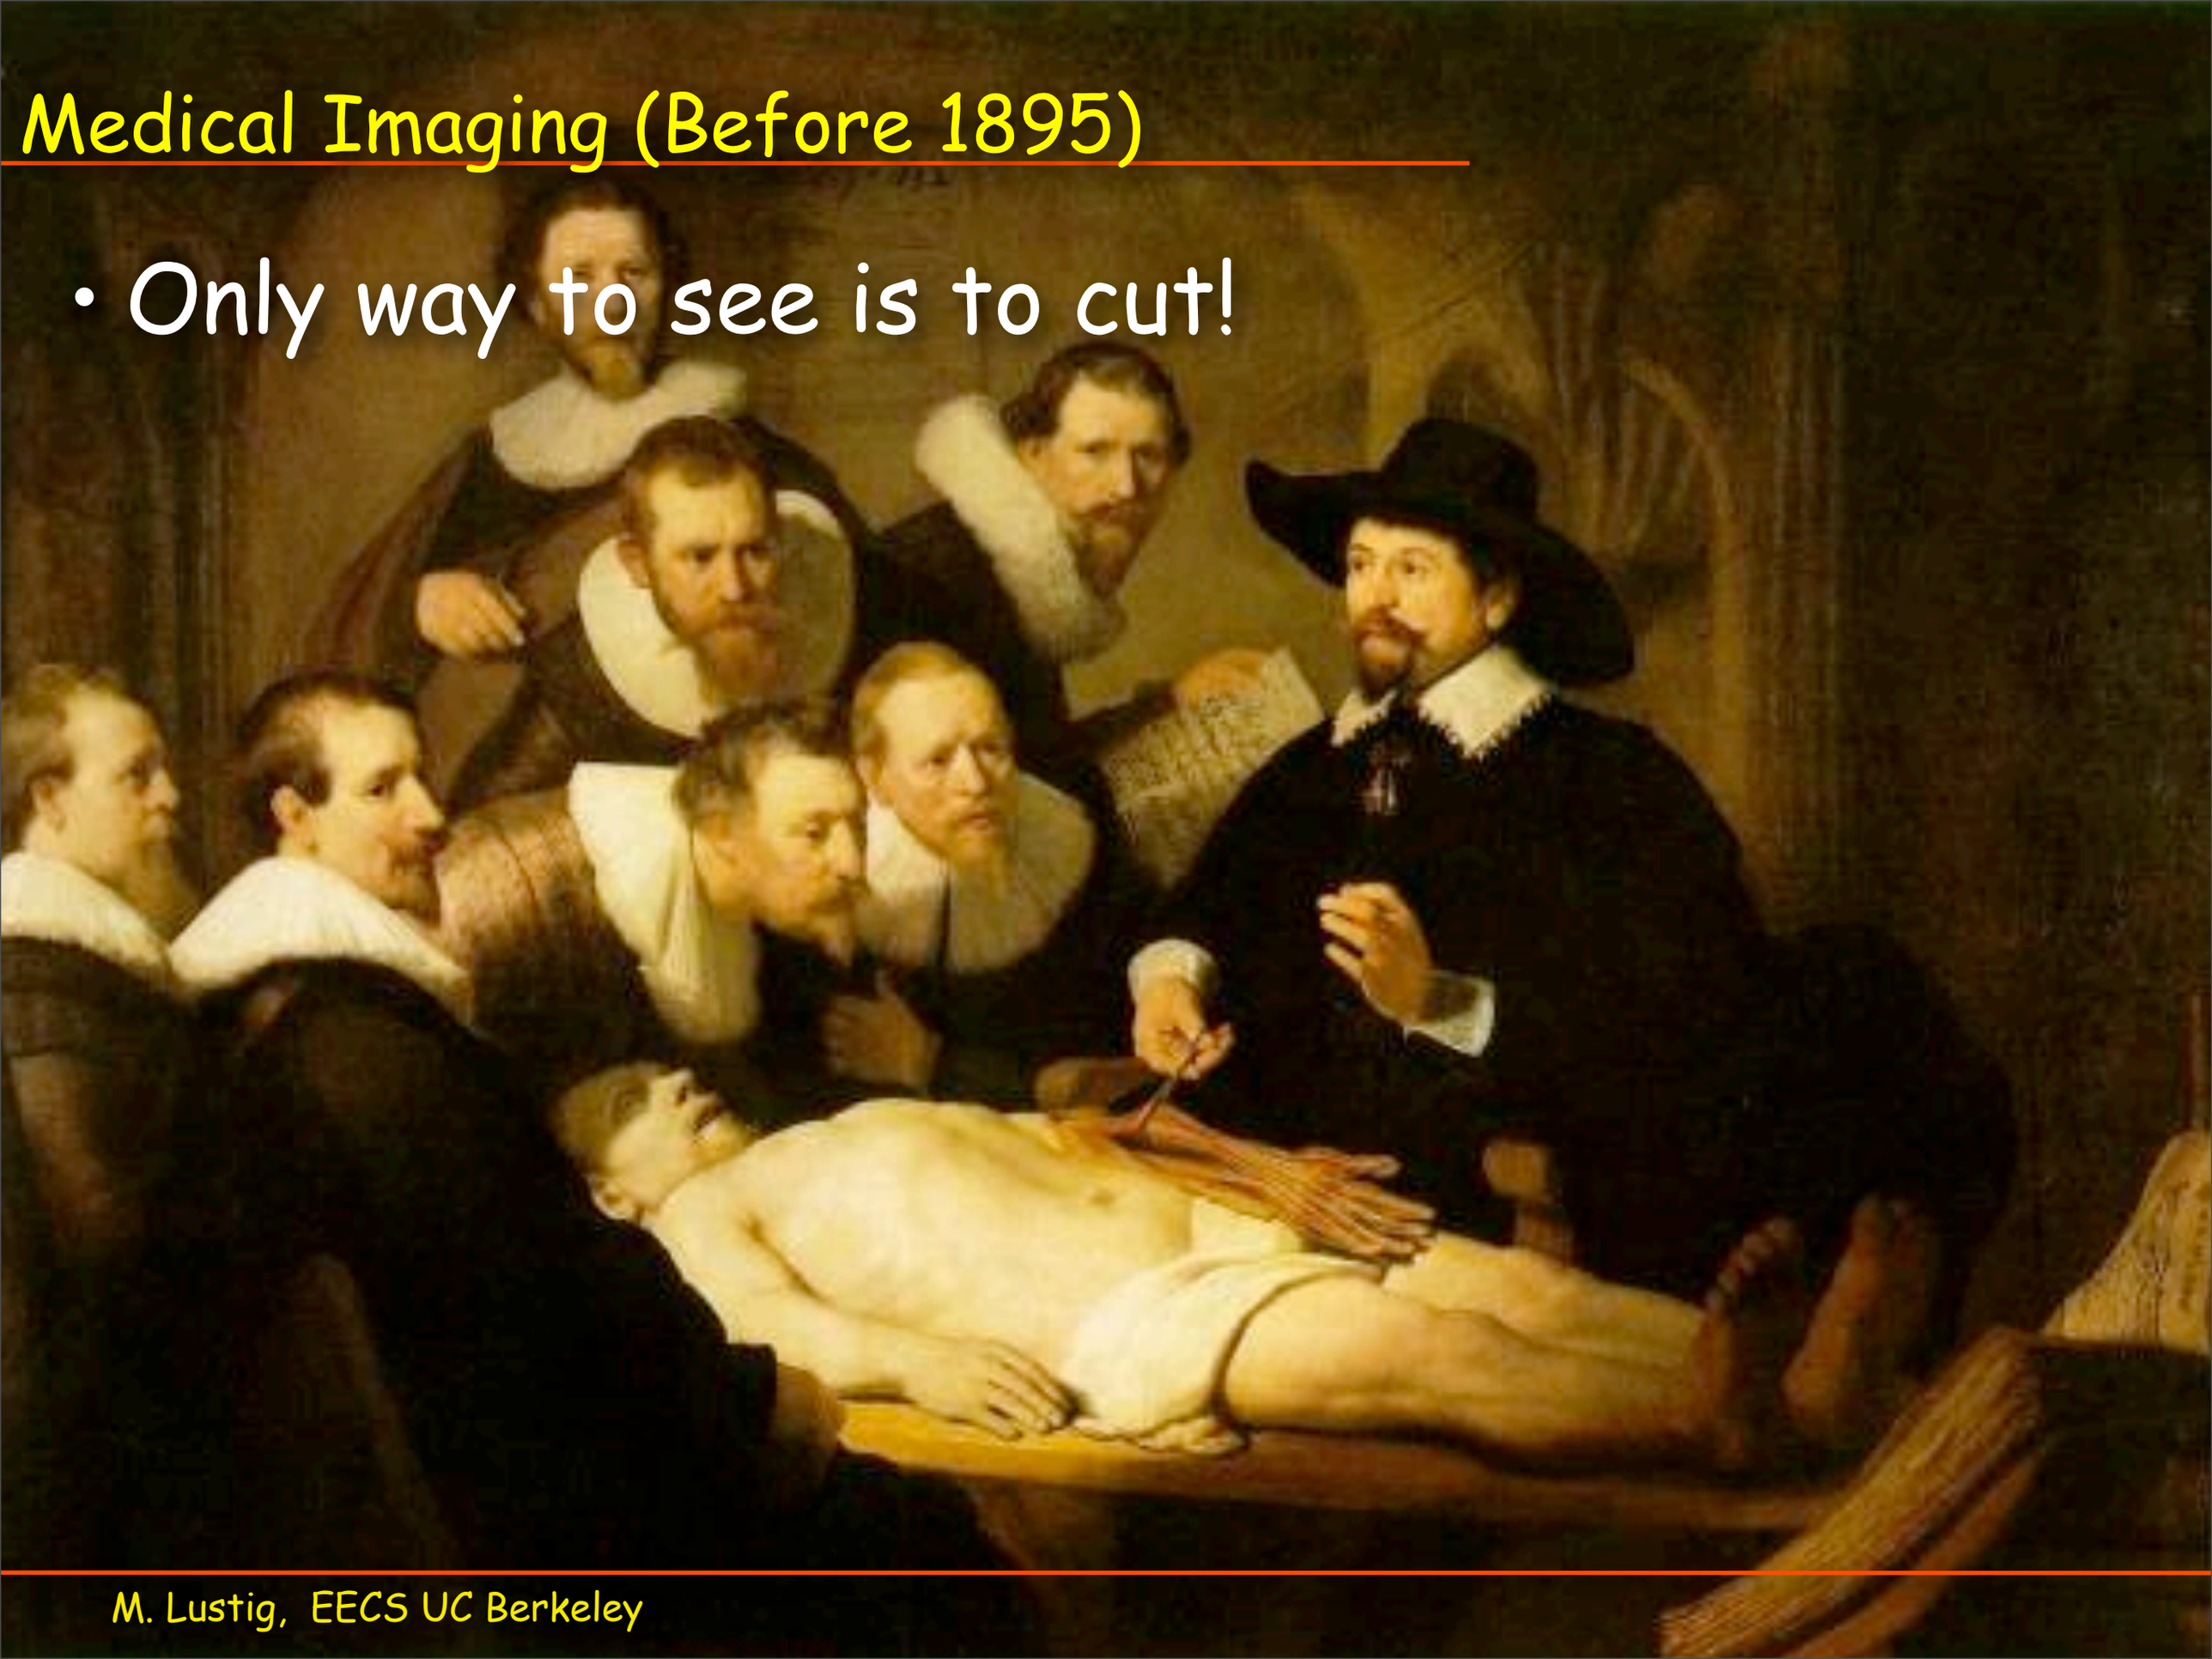

Medical Imaging (Post 1895)

- Revolutionized diagnostic medicine
- See internal anatomy
- Visualize function
- Many modalities
- Many sources of contrast

Basic Concept

Medical Imaging System Requirements

- Diagnostic contrast
- Sensitivity
- Specificity
- Function
- High Spatial-resolution
- High Temporal-resolution
- Safe
- Fast
- Inexpensive
- Easy to use
- Can't satisfy all
- Many modalities
- Often several used to make diagnosis

Common Imaging Modalities

- Projection X-Ray (Electromagnetic)
- Computed Tomography (Electromagnetic)
- UltraSound (Sound waves)
- Positron Emission Tomography (Nuclear)
- Single-Photon Emission Tomography (Nuclear)
- Magnetic Resonance Imaging (magnetic)

Medical Imaging is Multi-Disciplinary

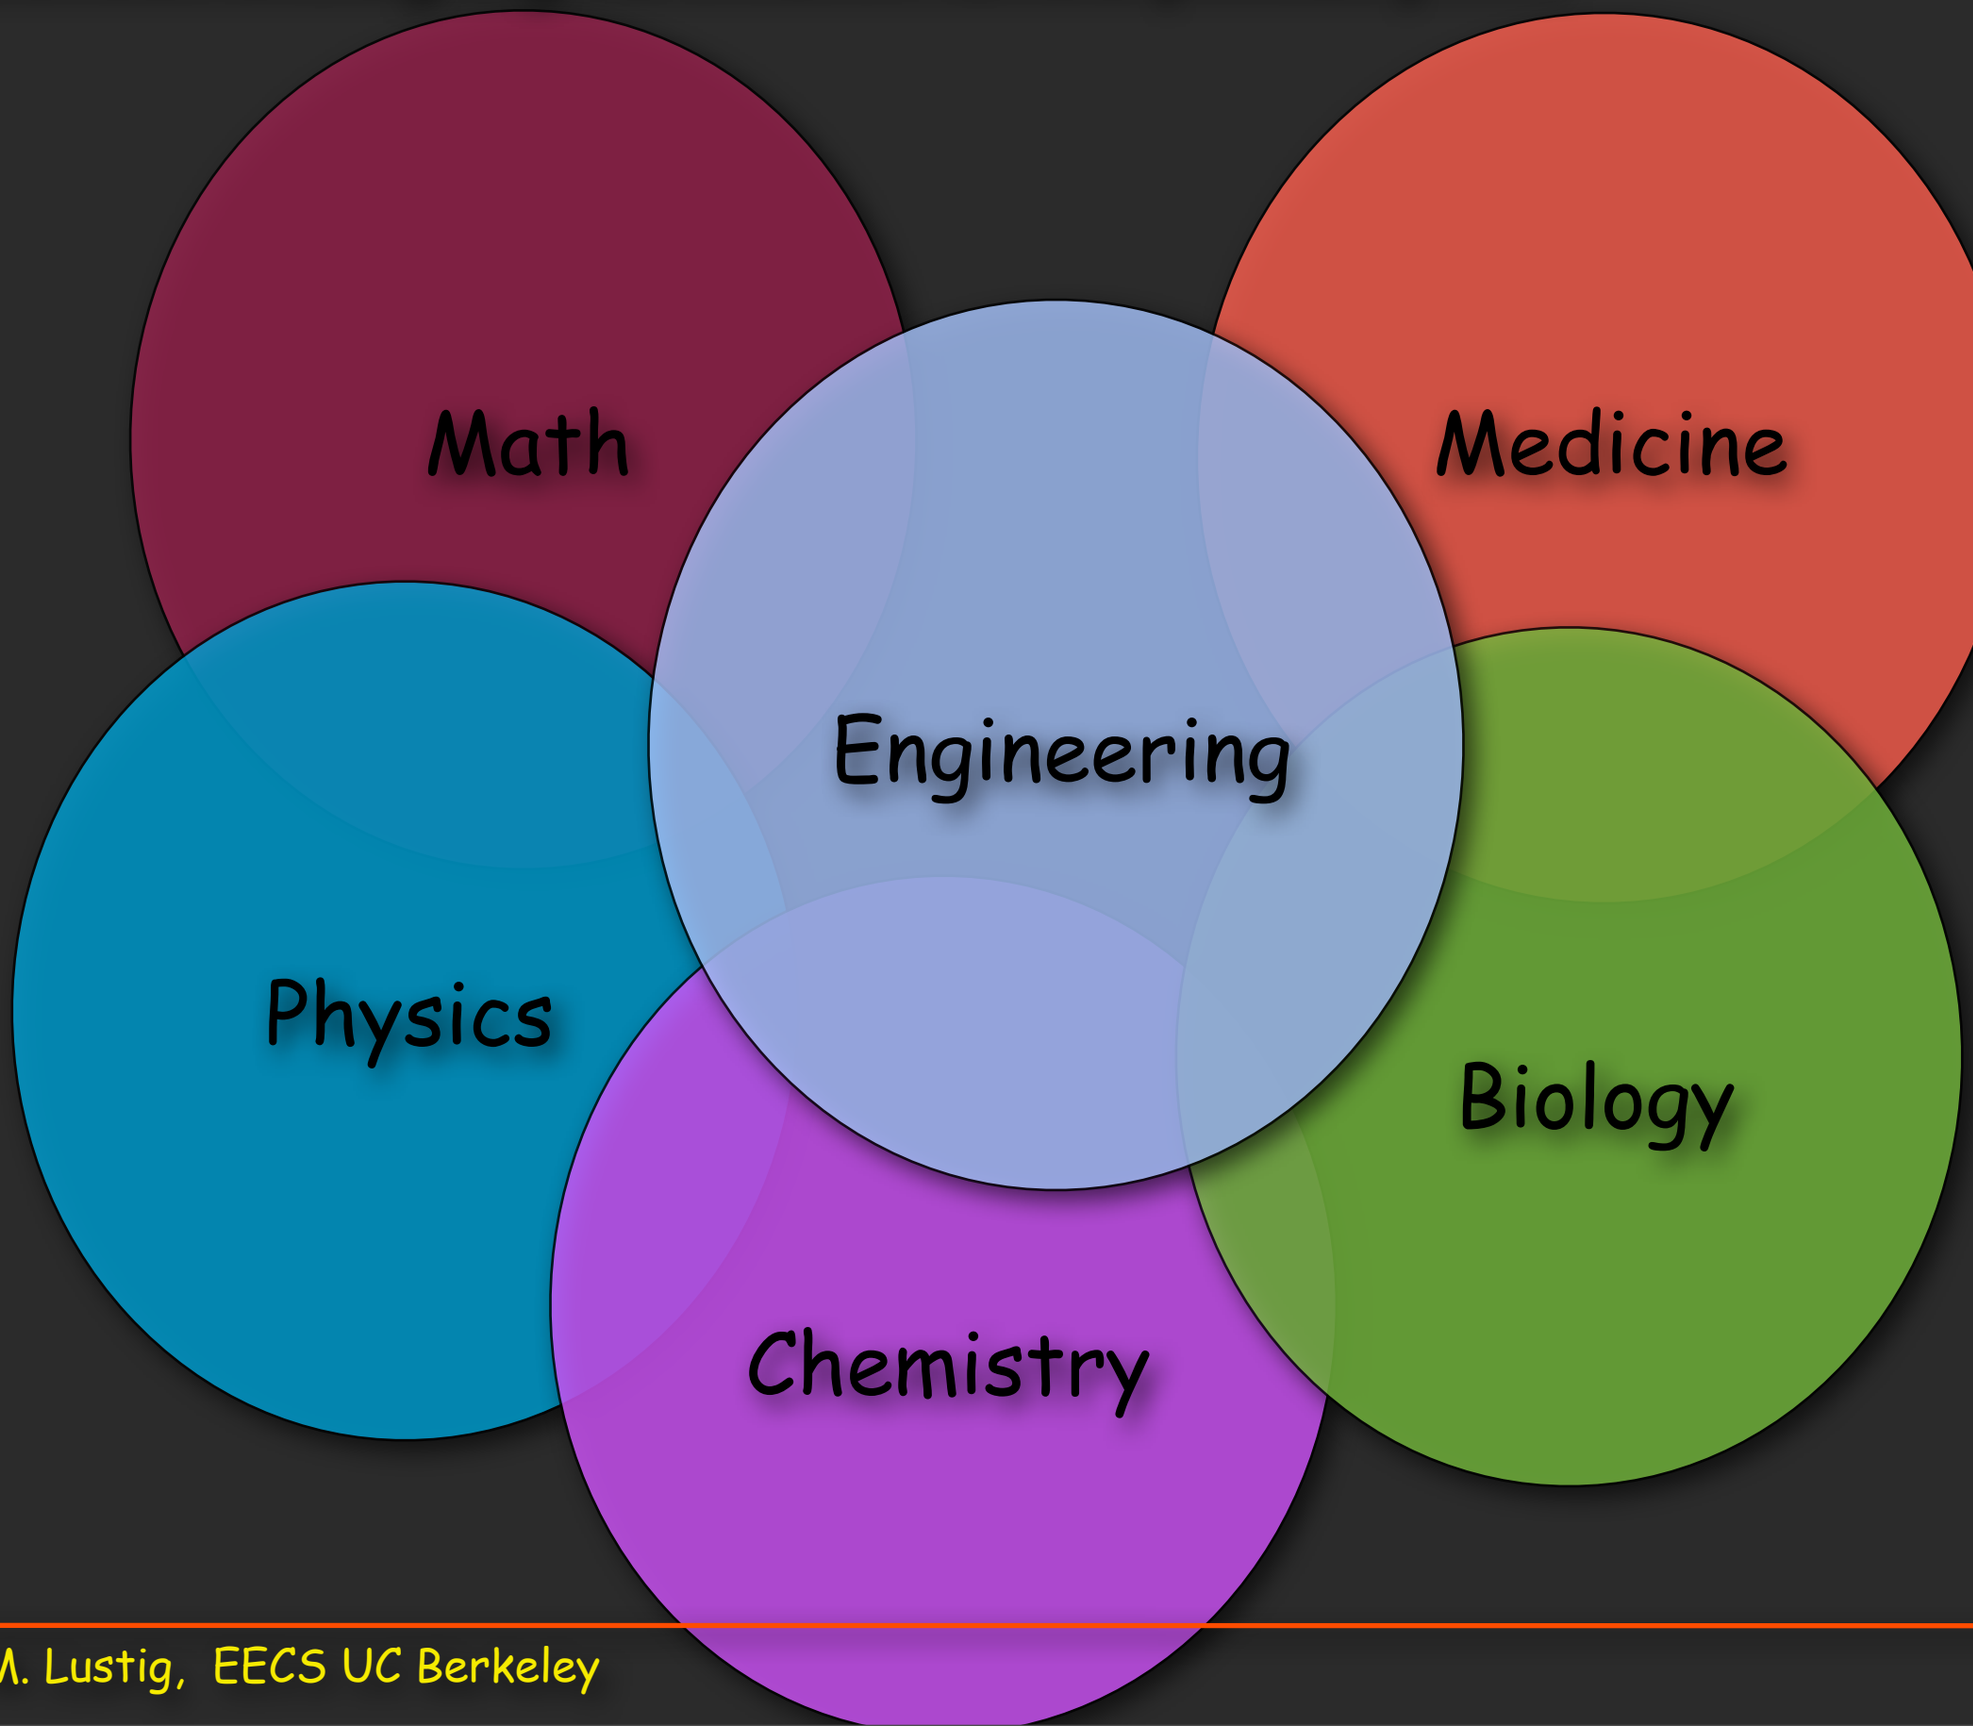

Engineering Advances

1st x-ray (1895)

x-ray today

Engineering Advances

early CT (1975)

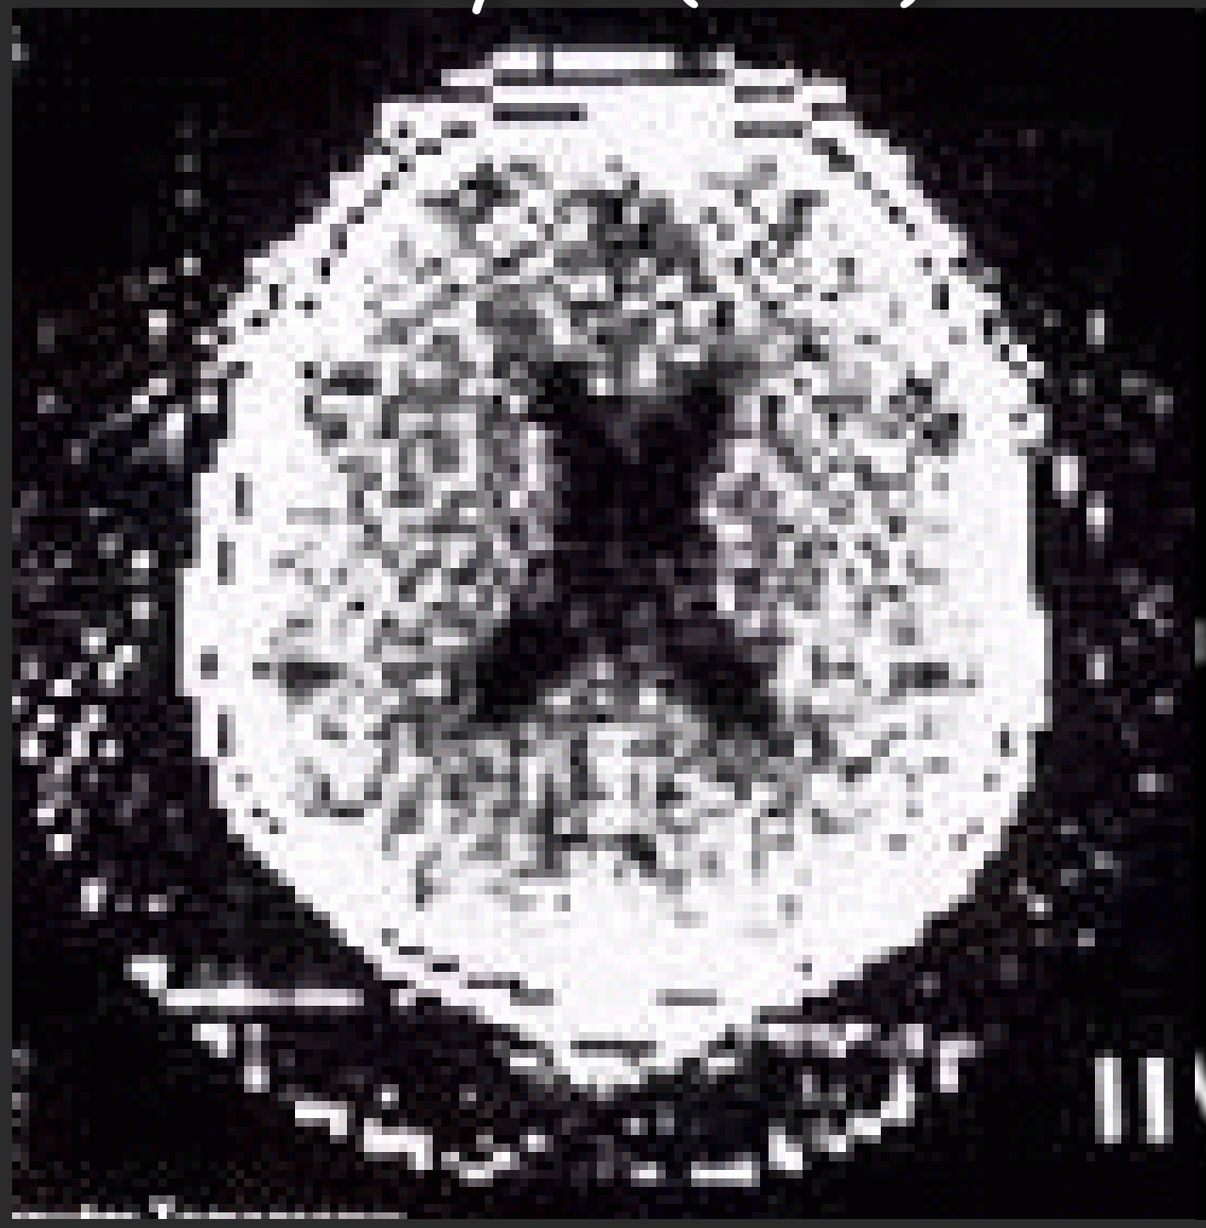

CT today

Engineering Advances

early ultrasound (1959)

ultrasound today

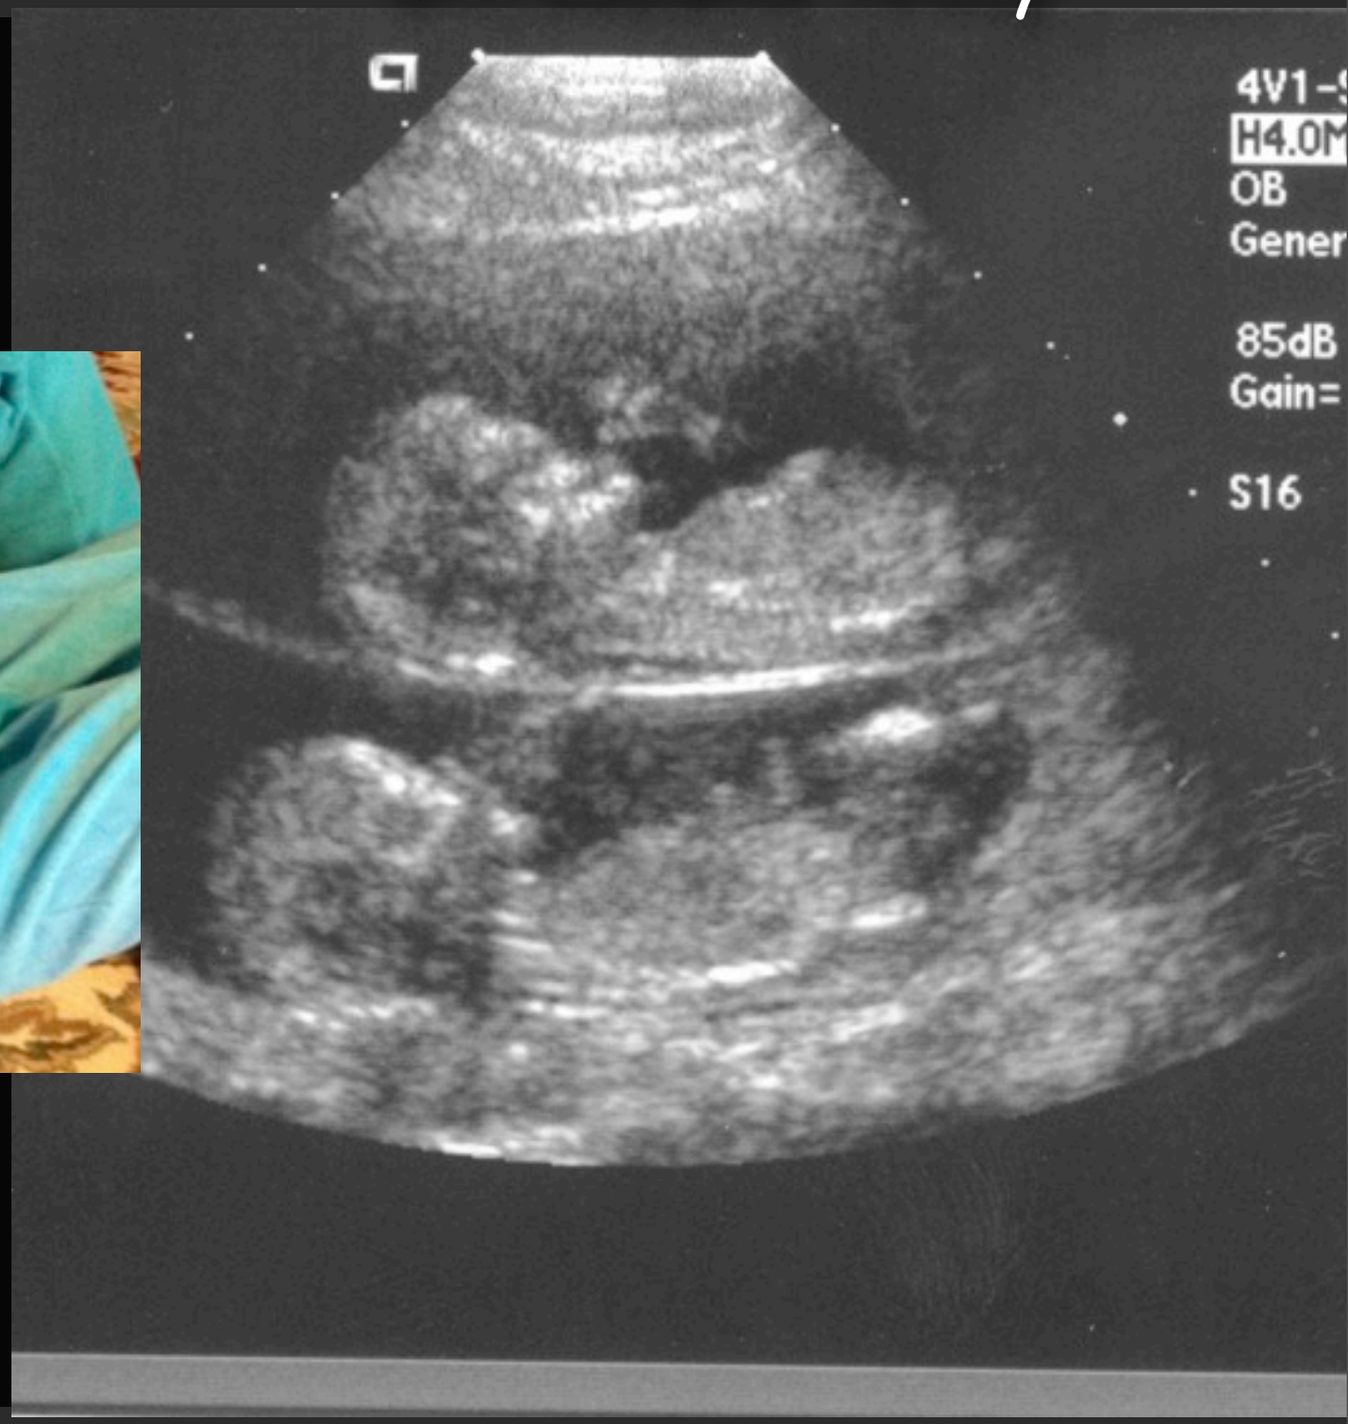

Engineering Advances

early MRI (1978)

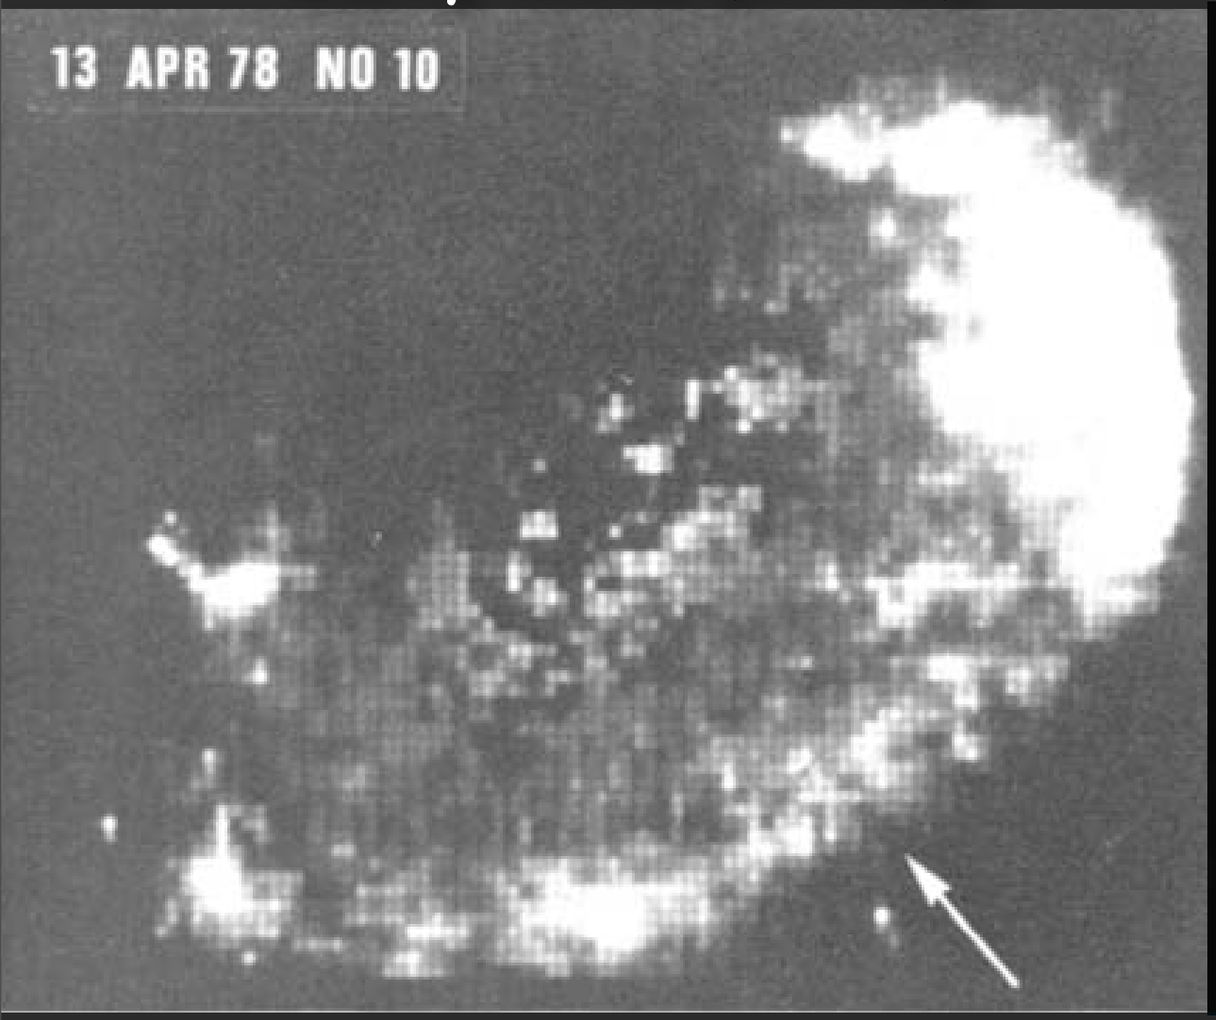

MRI today

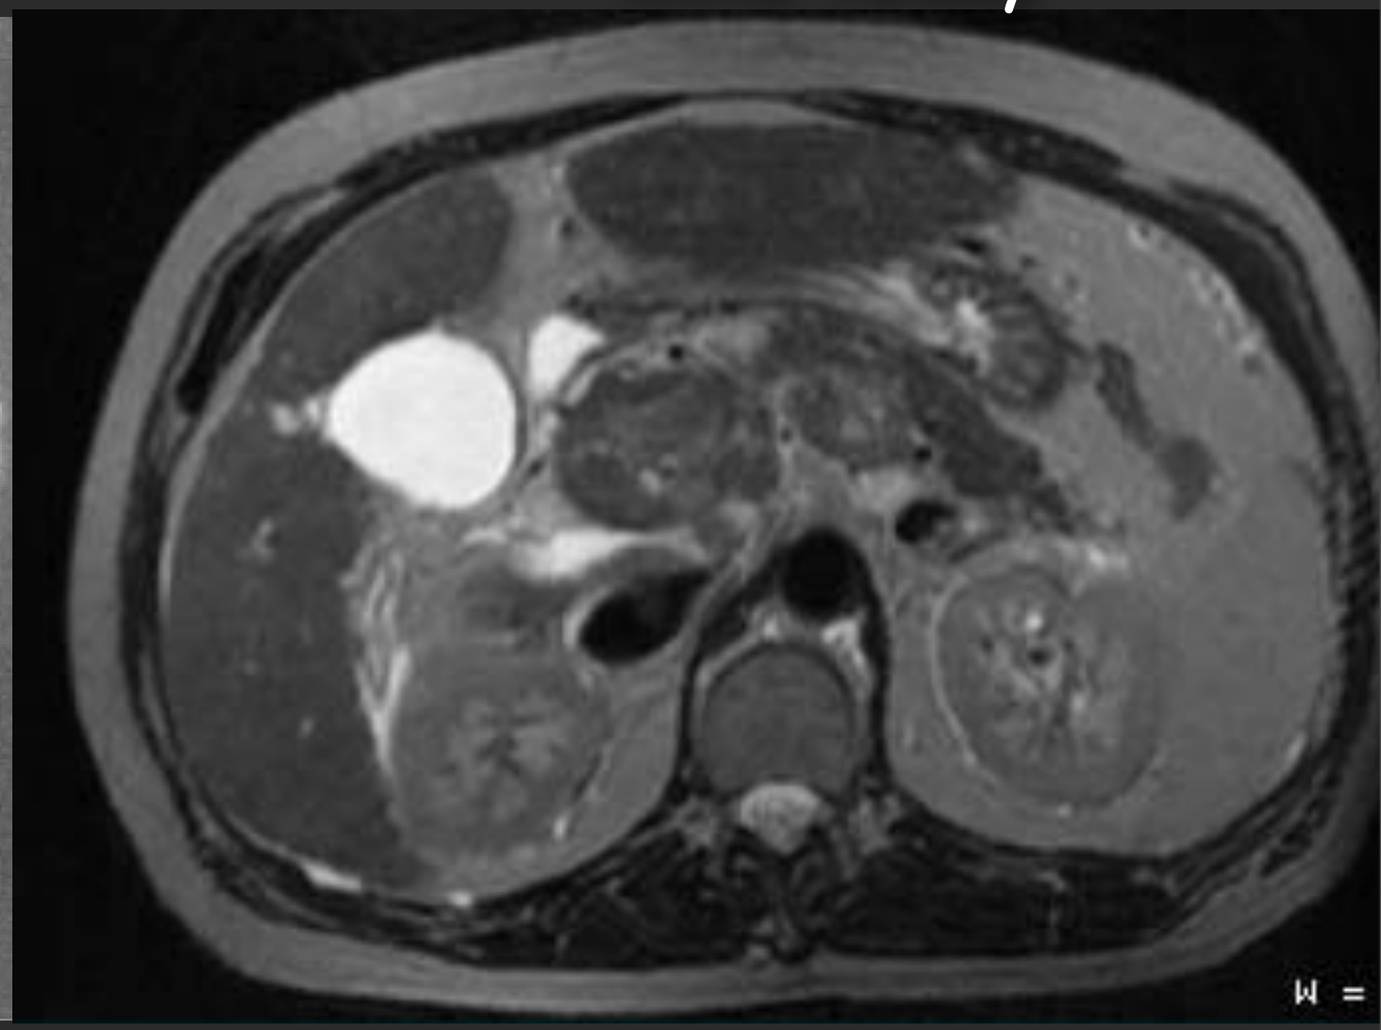

Projection X-Ray

- Projection Format
- Small Dose
- Fast
- Inexpensive

Projection

Computed Tomography (CT)

- Tomographic
- Fast
- High-Res
- Moderate dose
- ~1M$

Many Projections

Computed Tomography

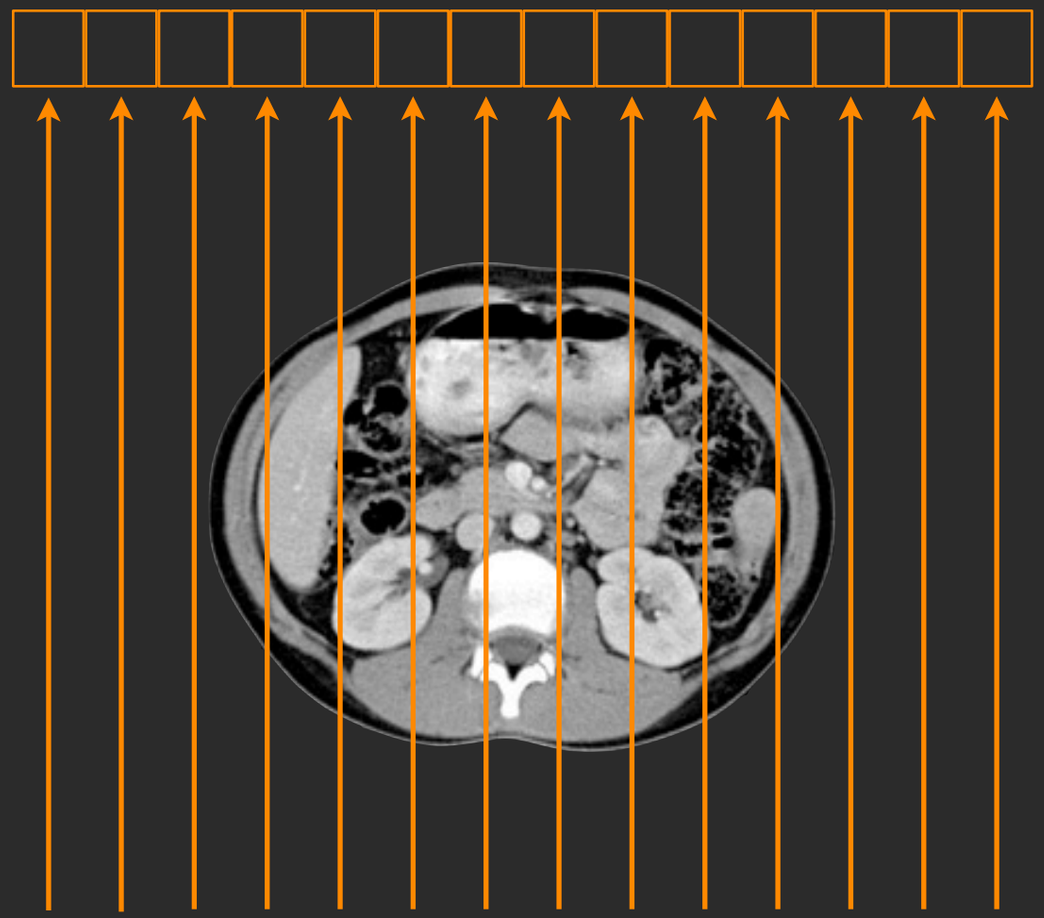

x-ray source

Sinogram

FBP

cross-section

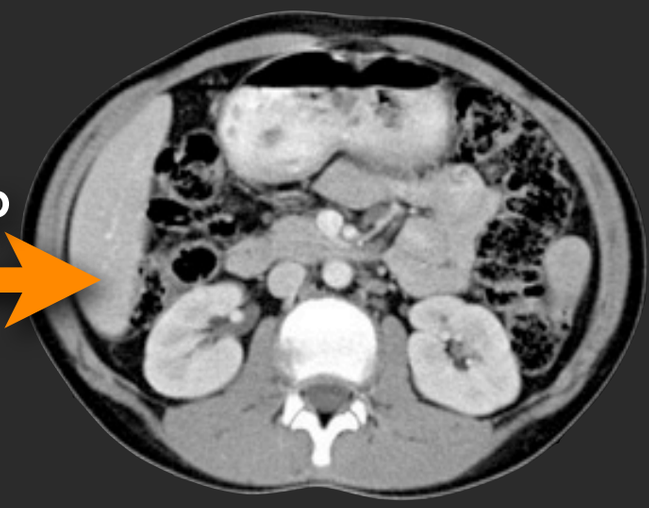

Computed Tomography

- Gantry rotation

M. Lustig, EECS UC Berkeley

http://www.youtube.com/watch?v=4gklQHM19aY&feature=related

Ultrasound

- Real-time
- Inexpensive
- No-radiation
- Many applications

- Low contrast and penetration

Echo

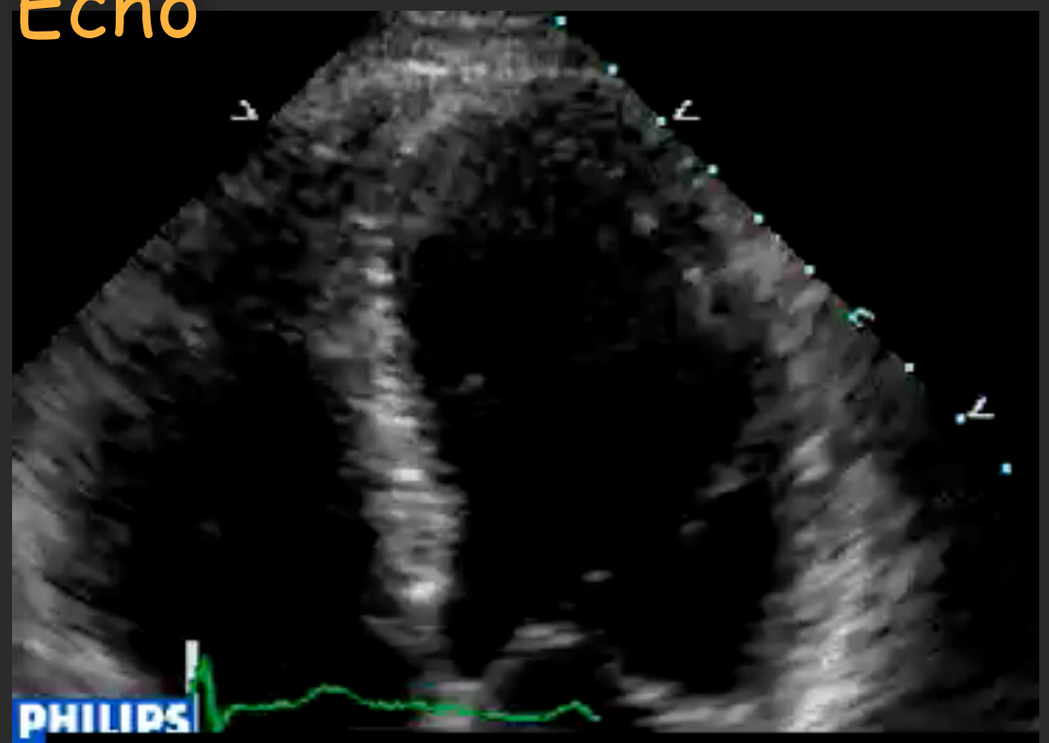

Anatomy vs Function

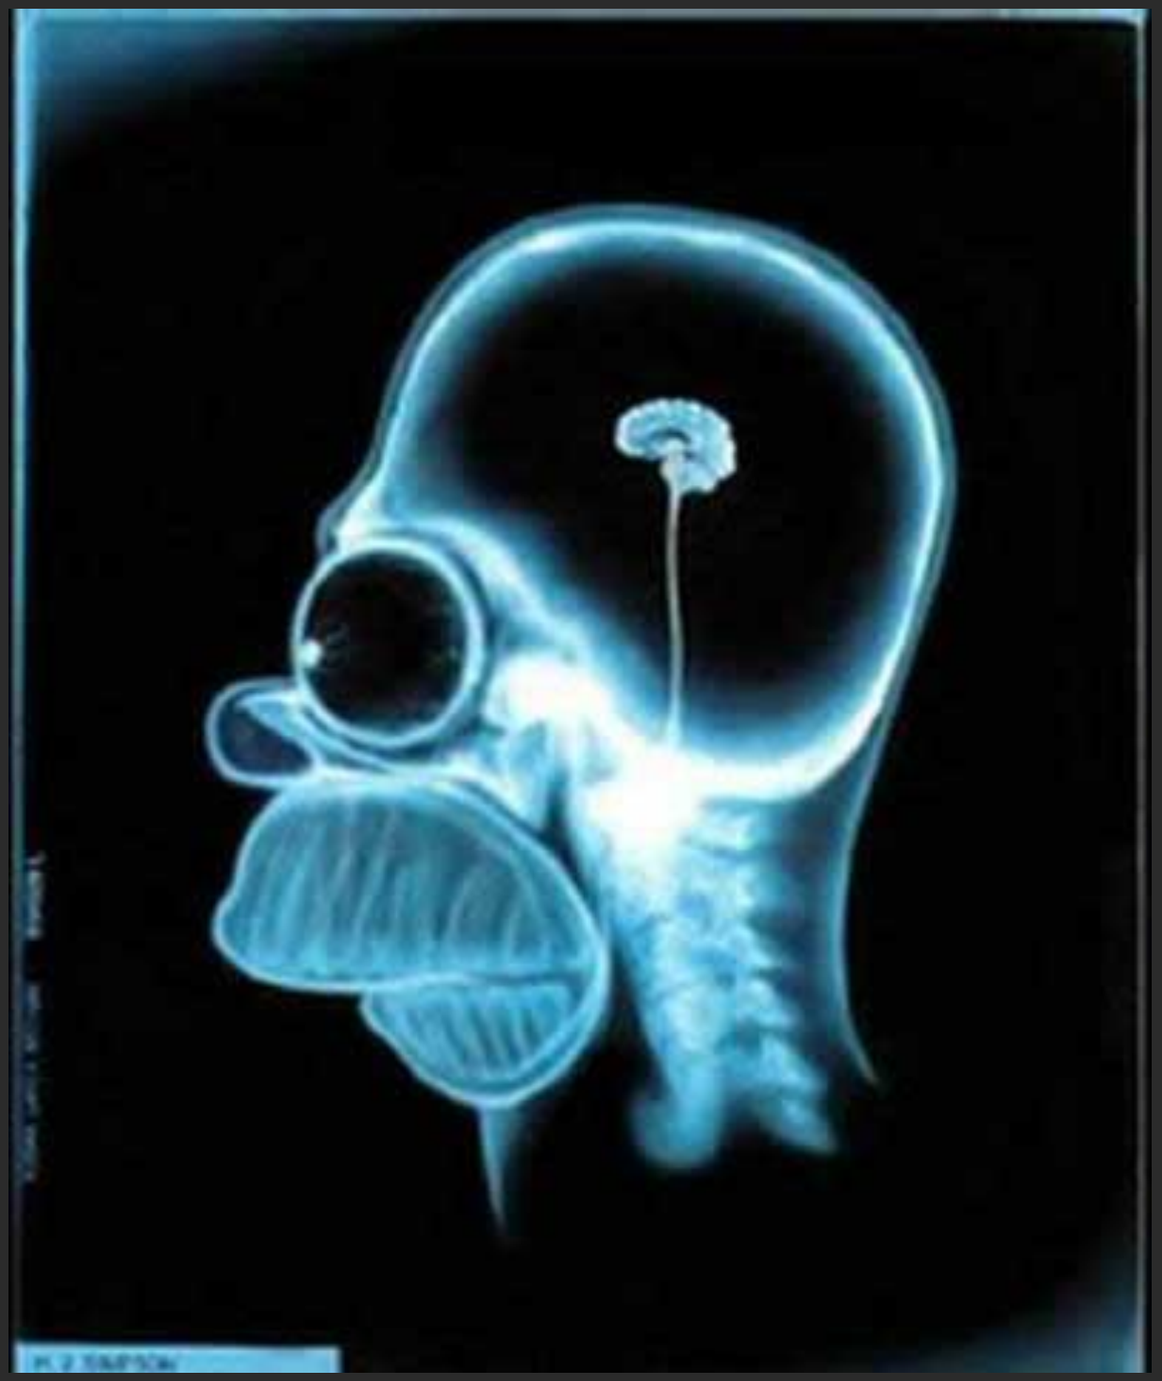

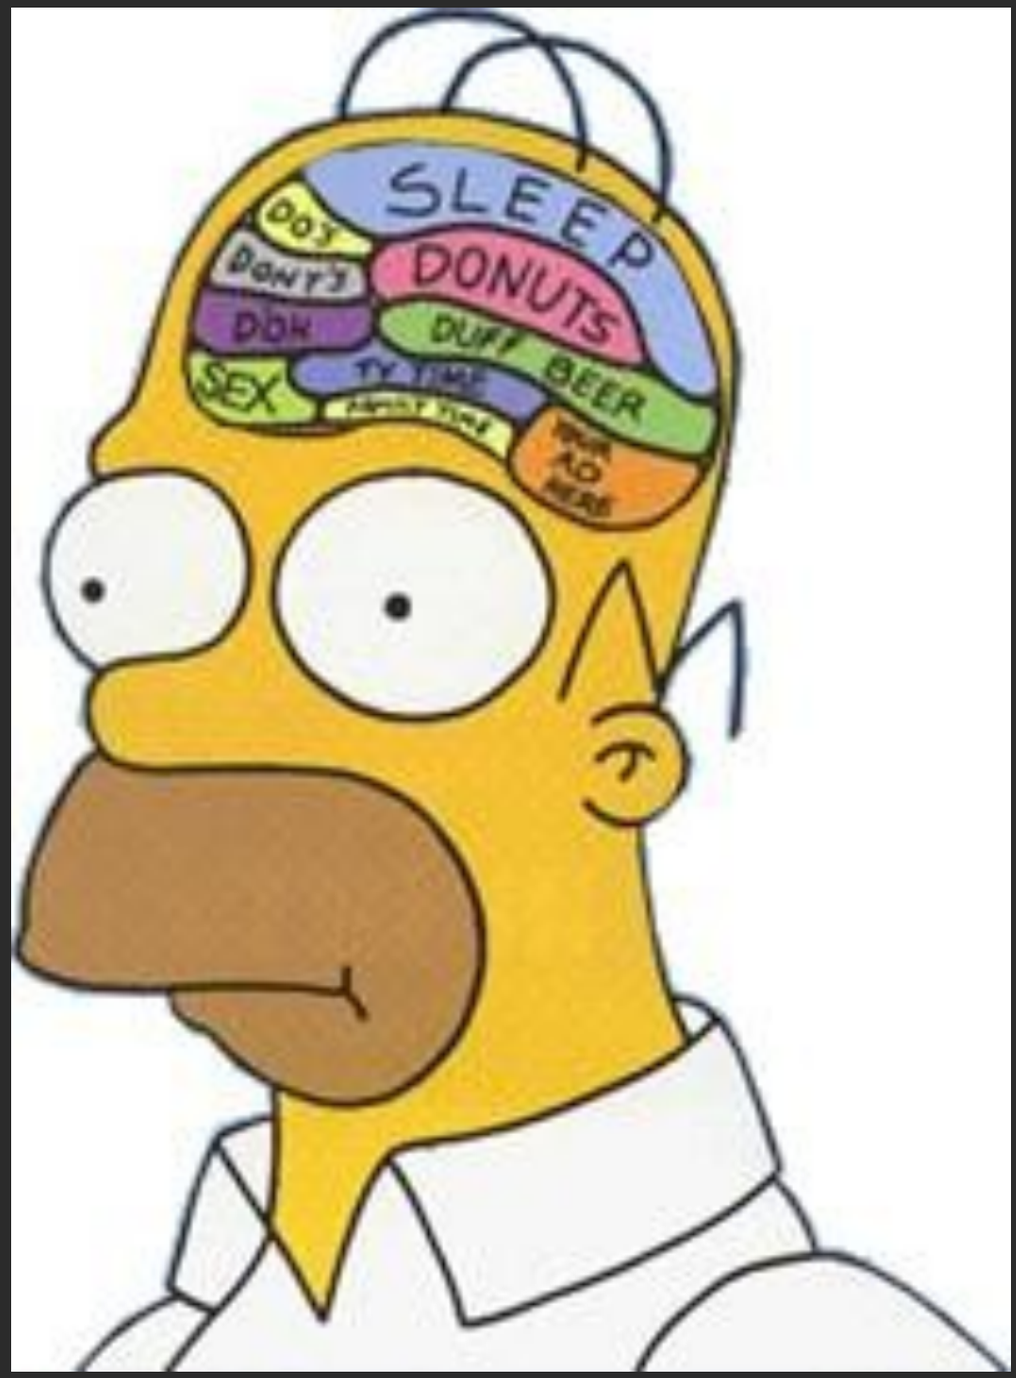

Nuclear Medicine

- Specific metabolic information (function)
- Low-res
- High dose
- 1-2M$

- SPECT: Gamma radiation
- PET: Positron-> Gamma

brain metabolism

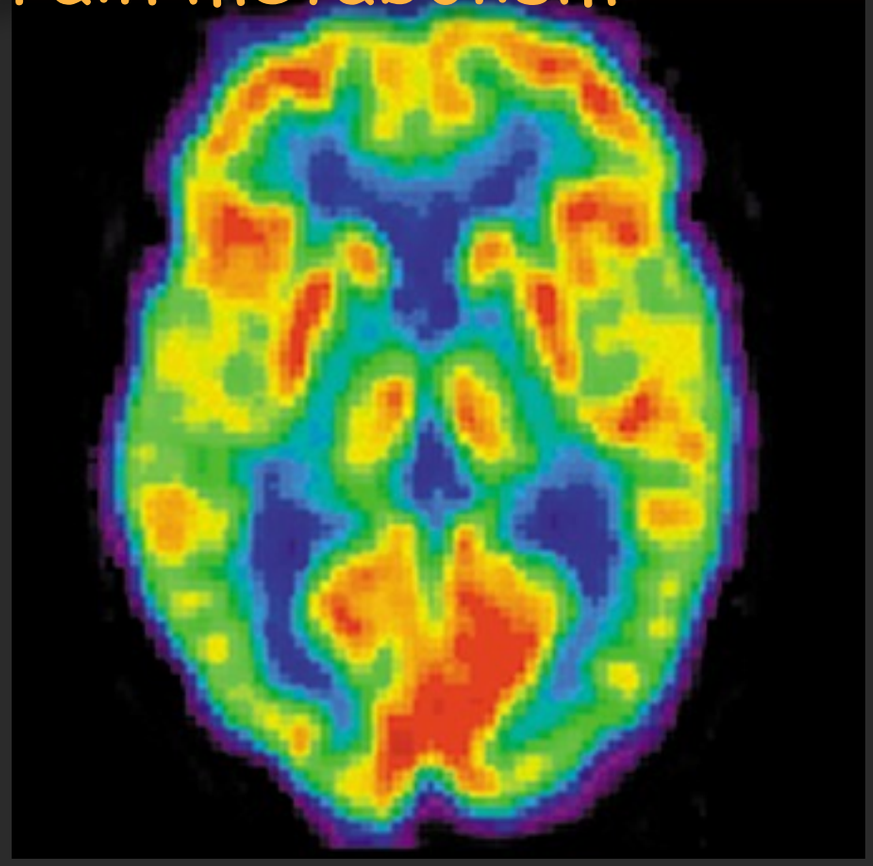

PET

Magnetic Resonance Imaging (MRI)

- NMR: Nuclear Magnetic Resonance
- MRI : Magnetic Resonance Imaging
  - please don't say MRI imaging!

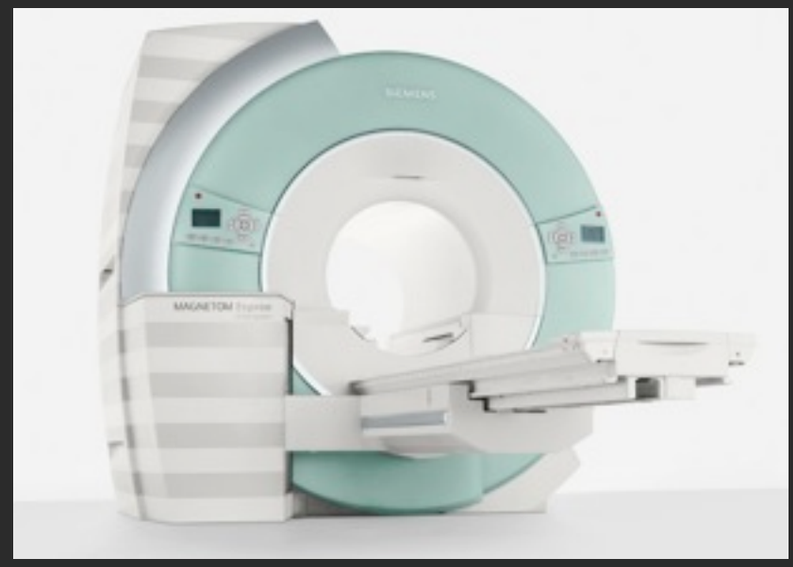

- MRI is VERY VERY VERY different from CT!
- Cost: 1M-3M, mainly because of the Magnet

History

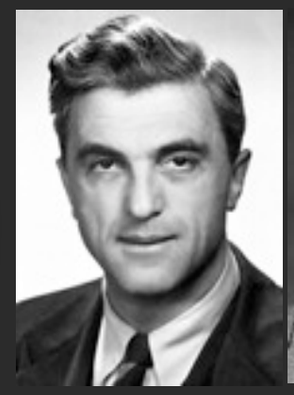


- 1946 - Felix Bloch (Stanford) Edward Purcell (Harvard) independently discovered NMR. Nobel Prize (Physics) in 1952.

- 1971 - Raymond Damadian showed changes in MR parameters (T1 and T2) in cancer. People started thinking about medical NMR applications.
- 1972 - Invention of CT by Hounsfield and Cormack. Nobel Prize (Medicine) in 1979.

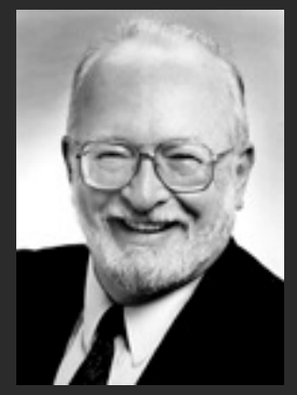

- 1973 - Lauterbur described MRI in a similar way to CT

History

- 1975 - Ernst proposed key concepts. Nobel prize (Chemistry) 1991.
- 1970's - Mansfield contributes key ideas (slice selection)
- 1982 - Widespread clinical MRI begins.
- 2003 - Lauterbur/Mansfield receive Nobel prize (Medicine) for their contributions.

MR Imaging

- Magnetic resonance imaging has revolutionized medicine
- Directly visualizes soft tissues in 3D
- Wide range of contrast mechanisms
  - Tissue character (solid, soft, liquid, fat, ...)
  - Diffusion
  - Temperature
  - Flow, velocity
  - Oxygen Saturation

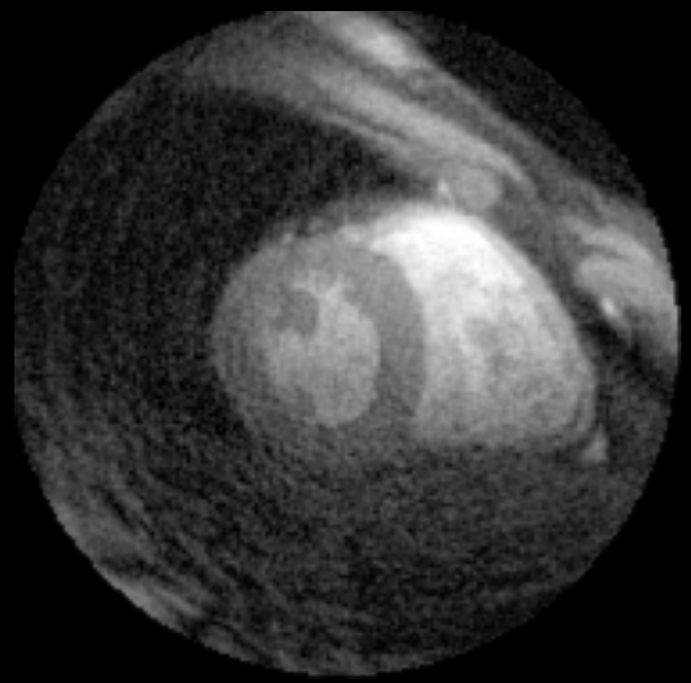

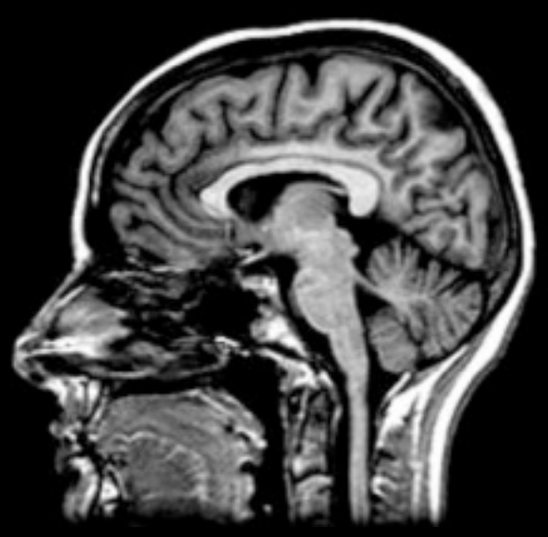

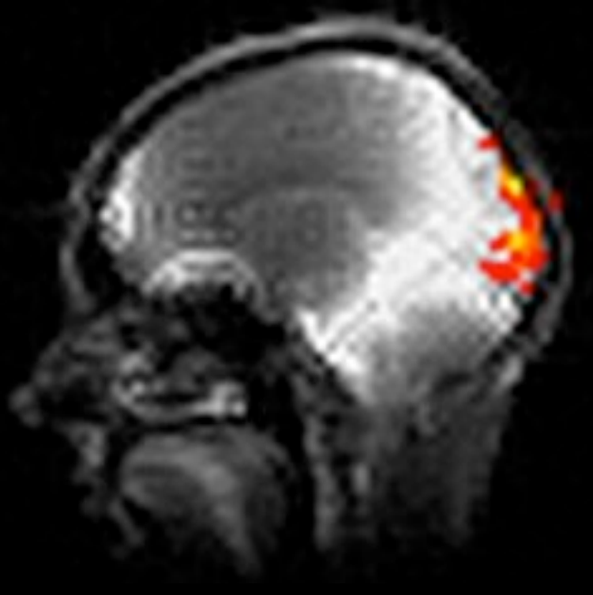

Neuro Examples

PD

T1

T2

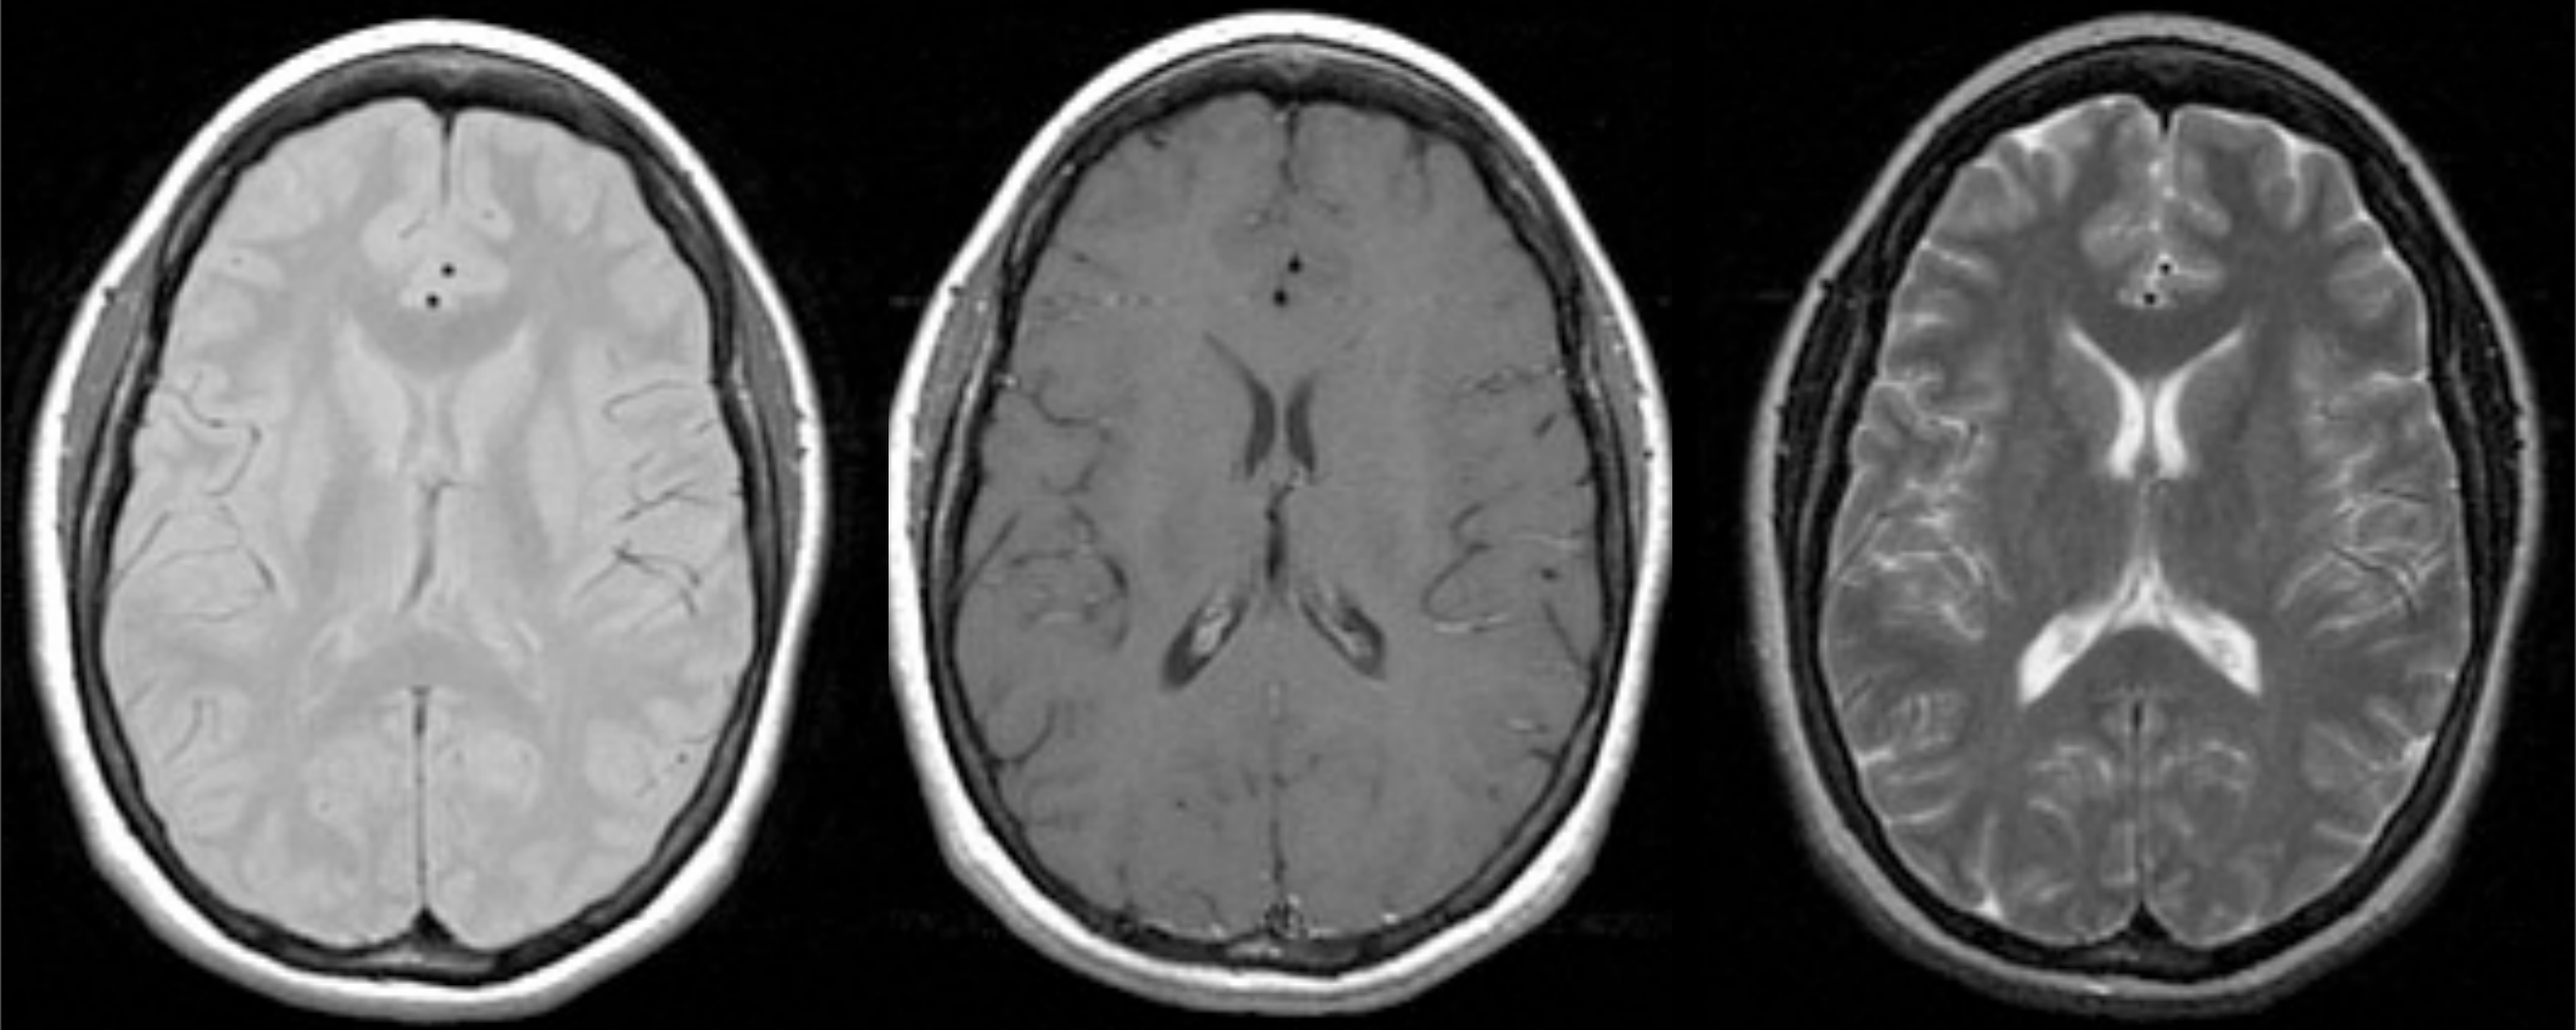

Many different contrasts available

Clinical Example

No Contrast Agent

Contrast Agent

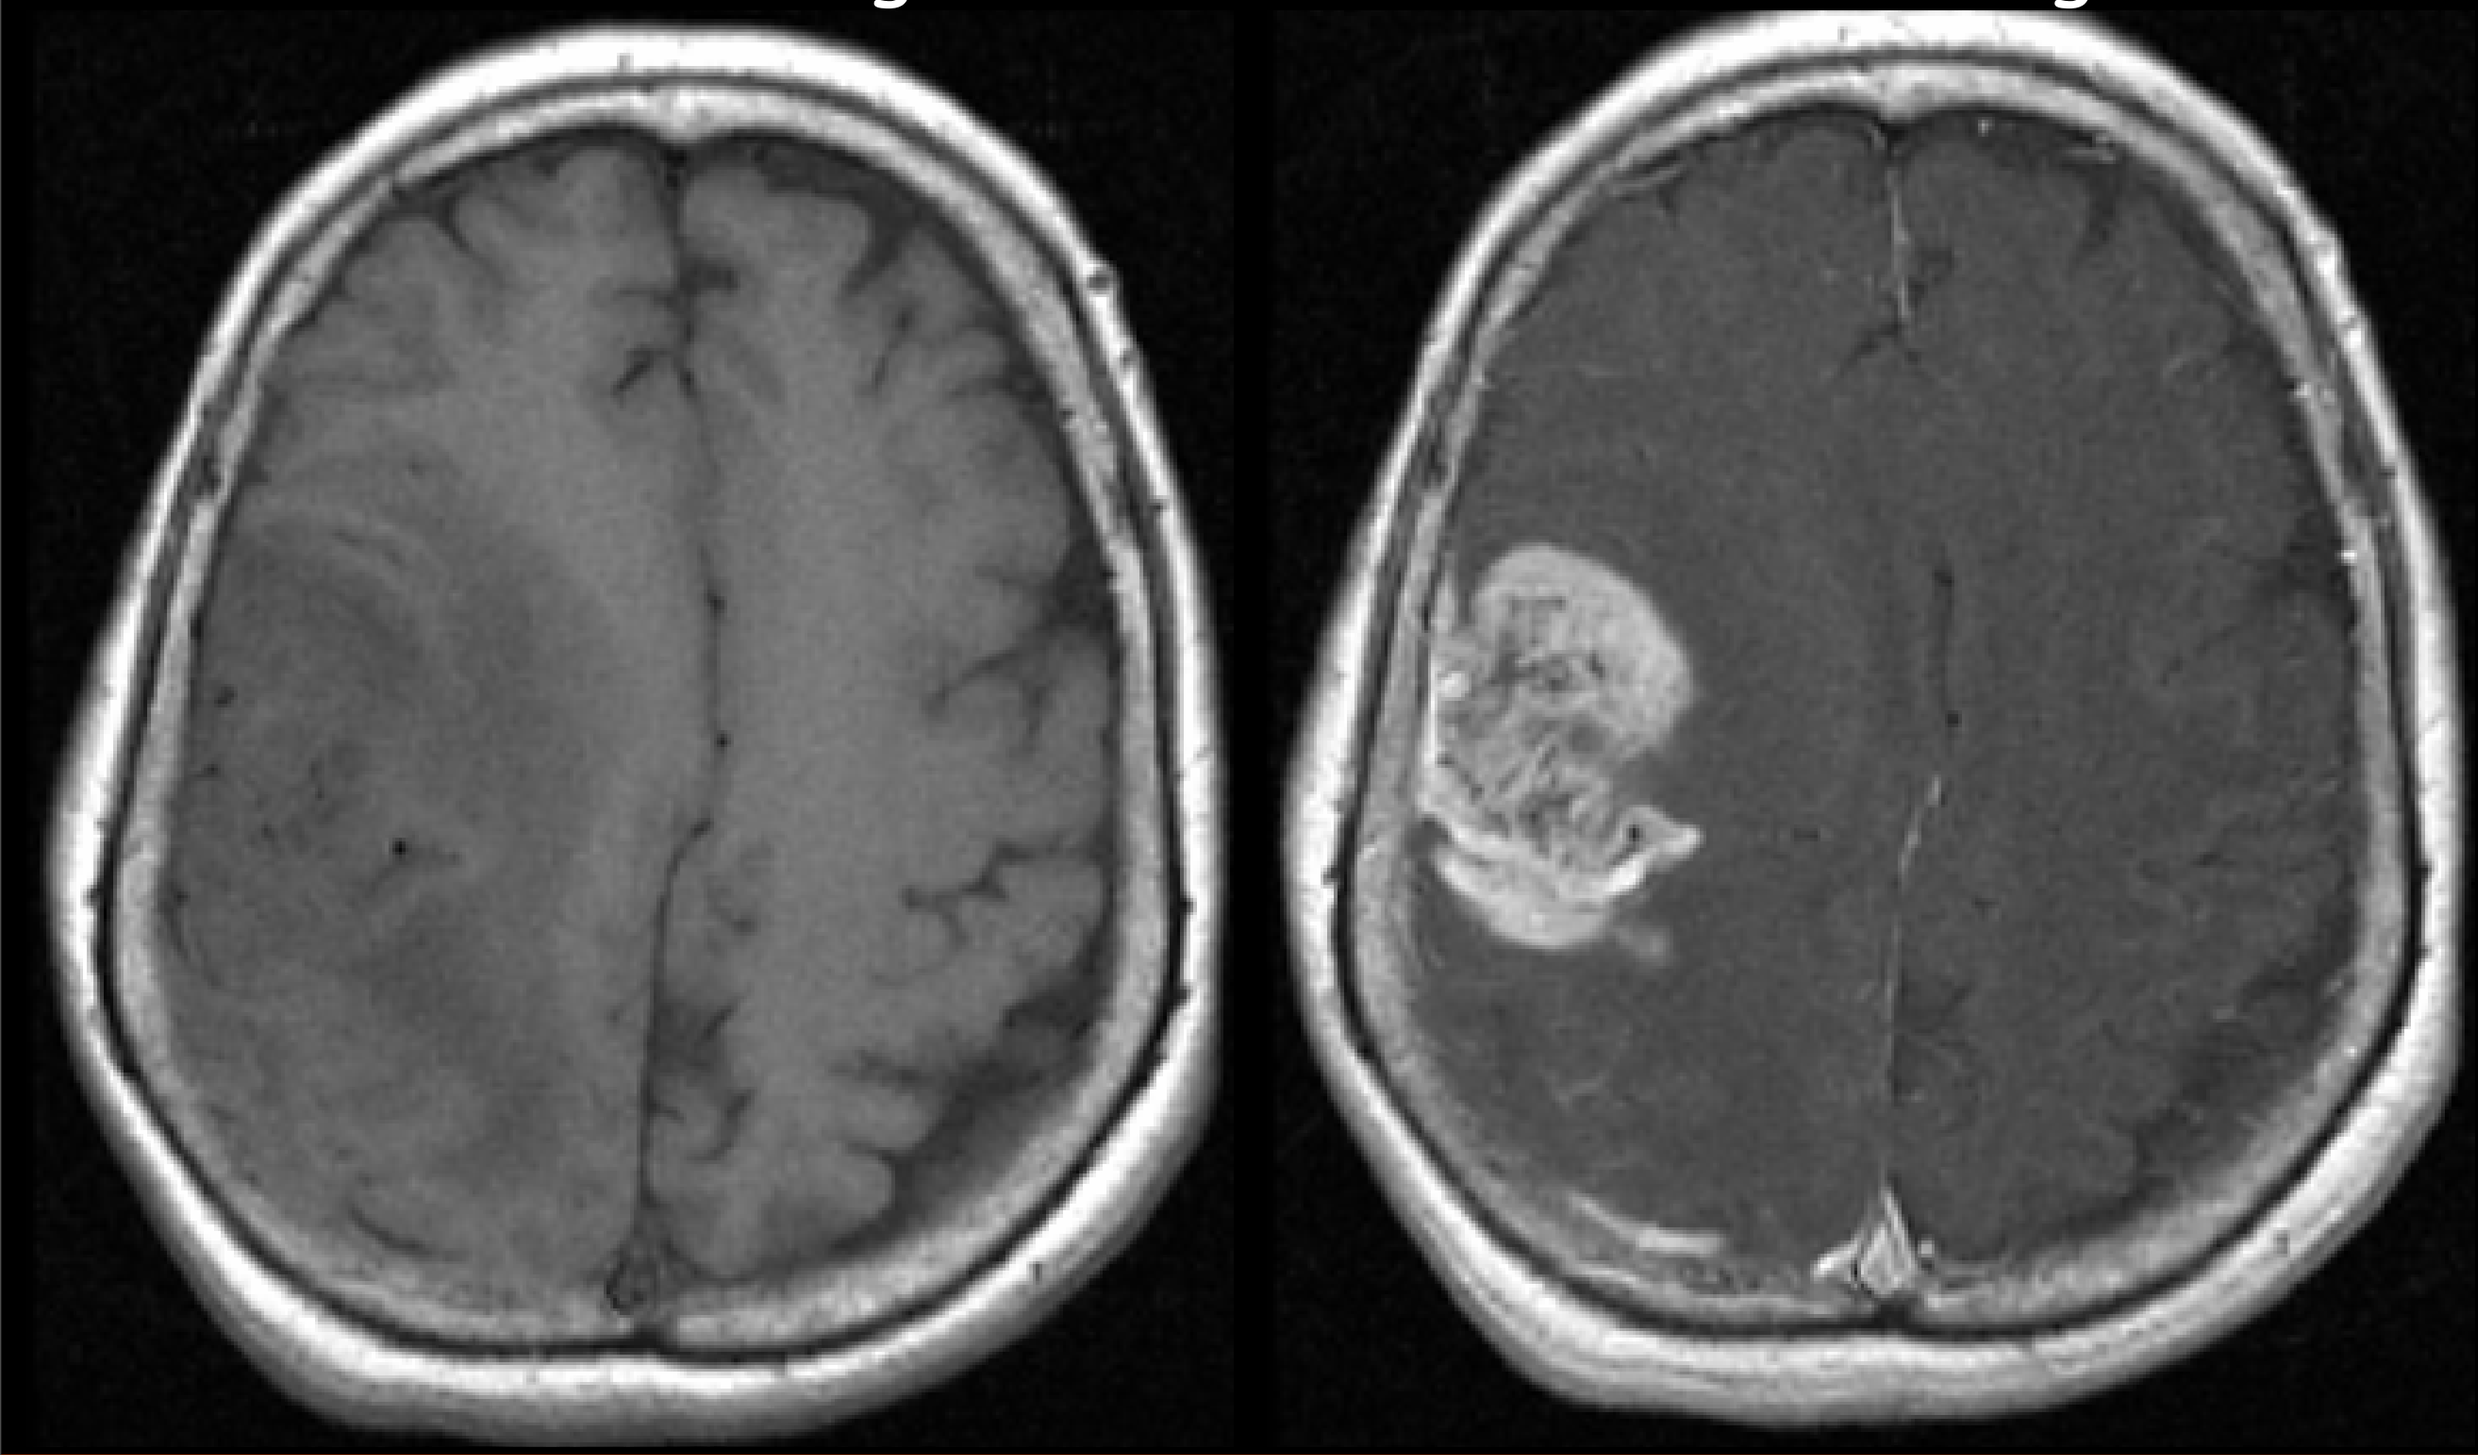

*K. Pauly, G. Gold, RAD220

Body Examples

Abdominal Blood Vessels

Knee

Angiography

contrast dynamics

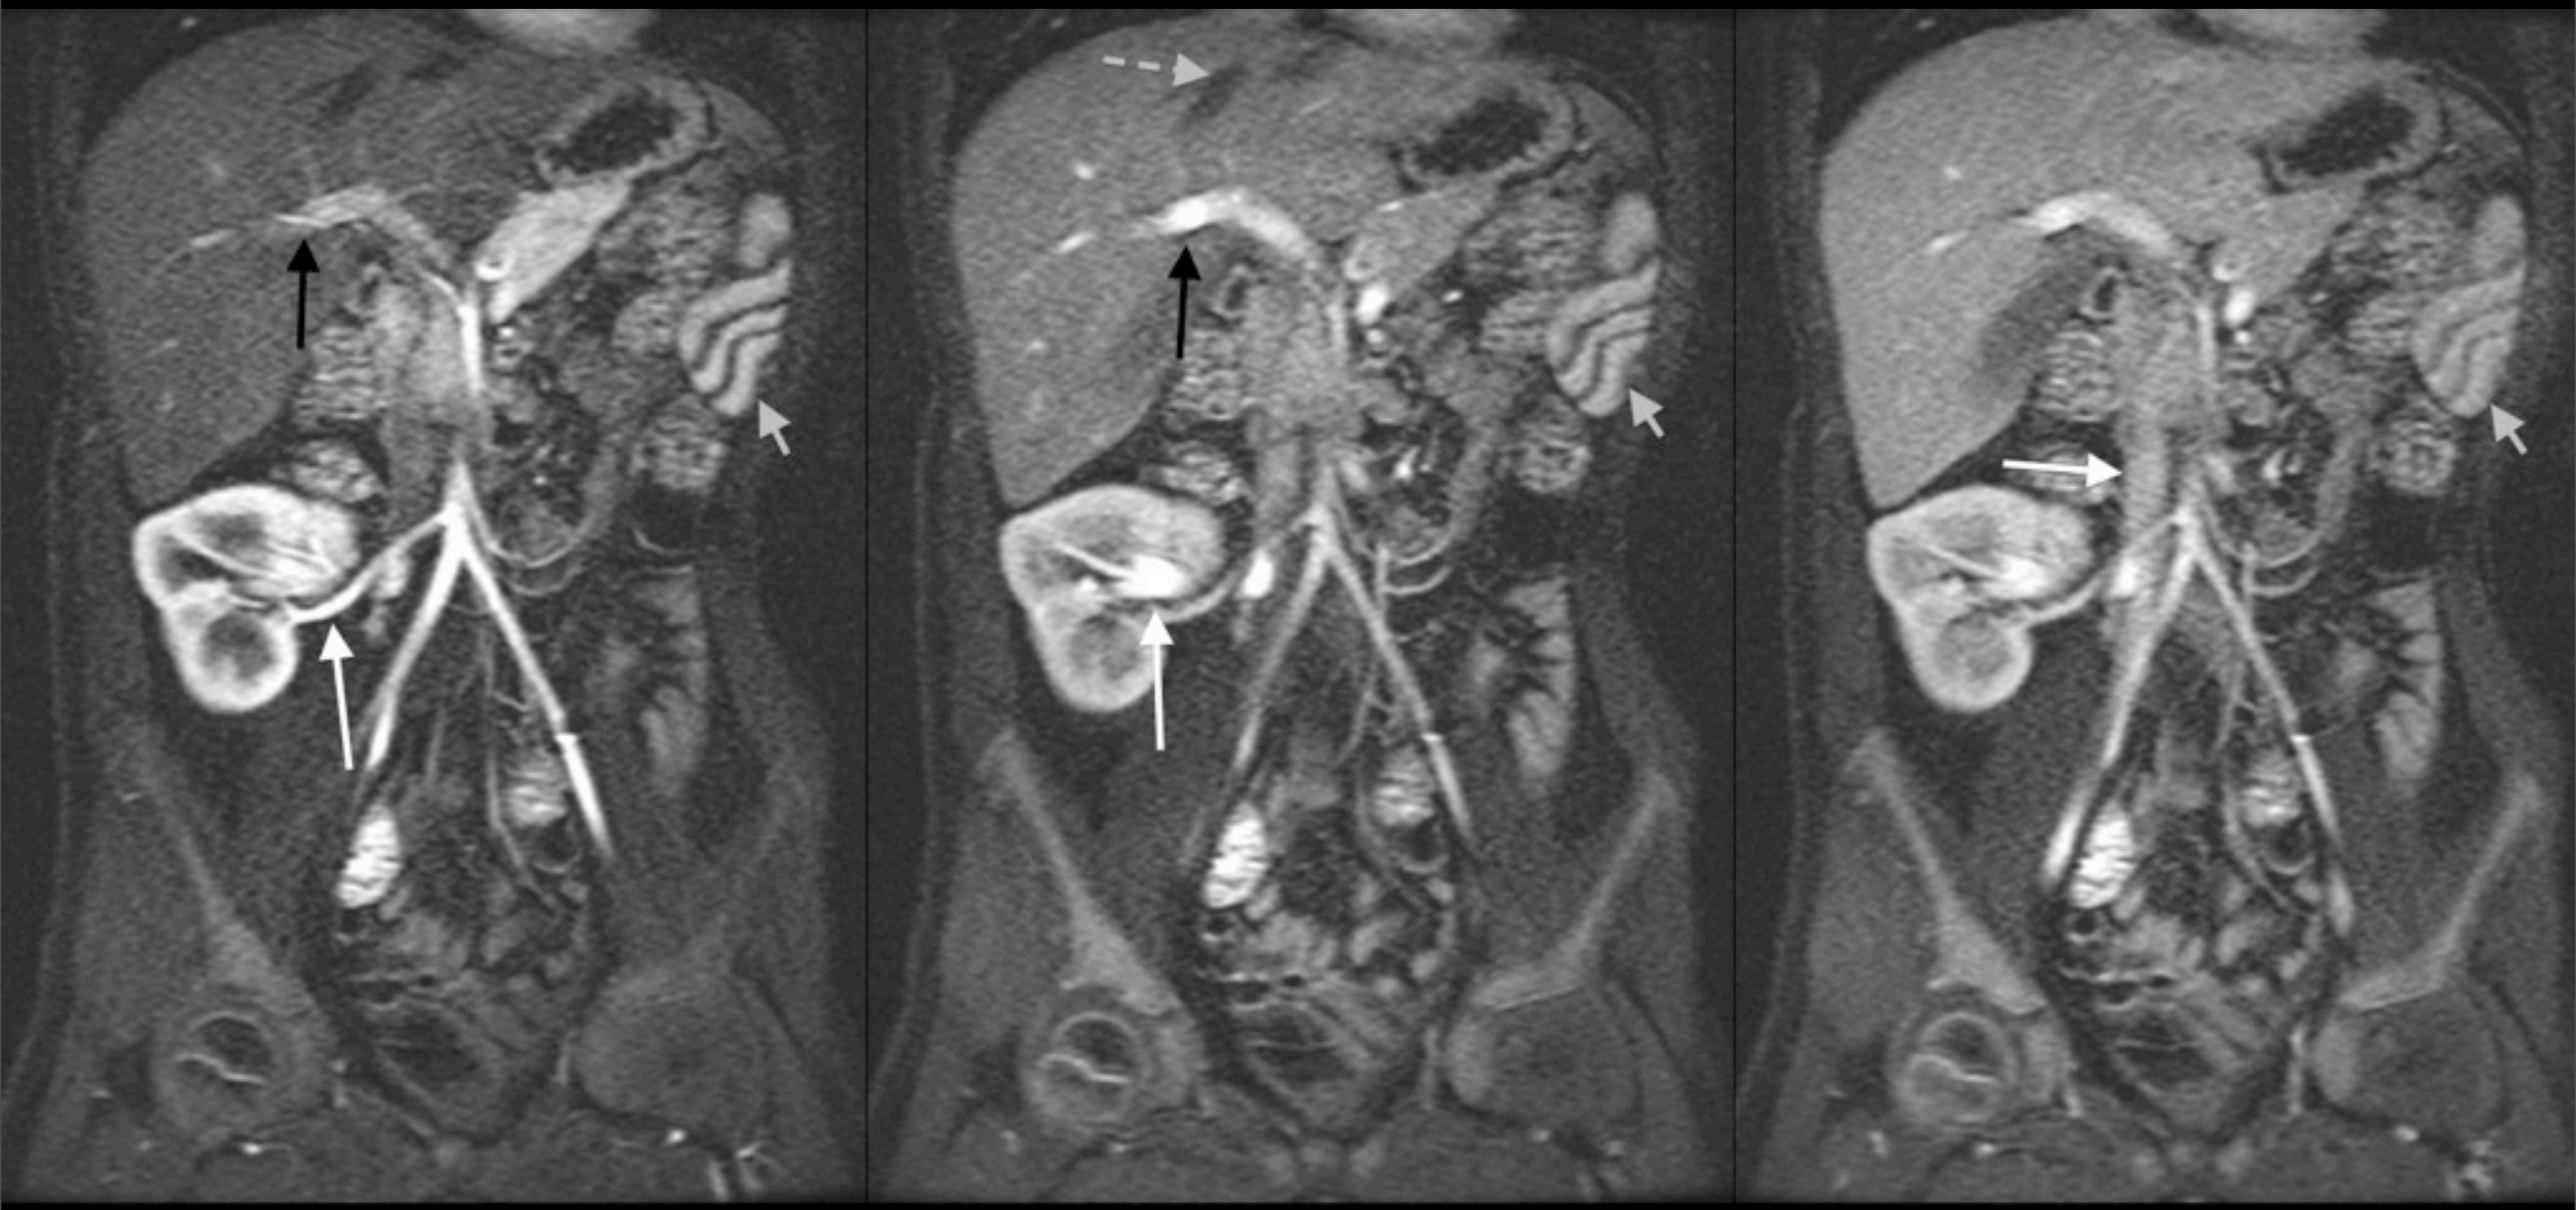

Cardiac MRI

gated

real-time

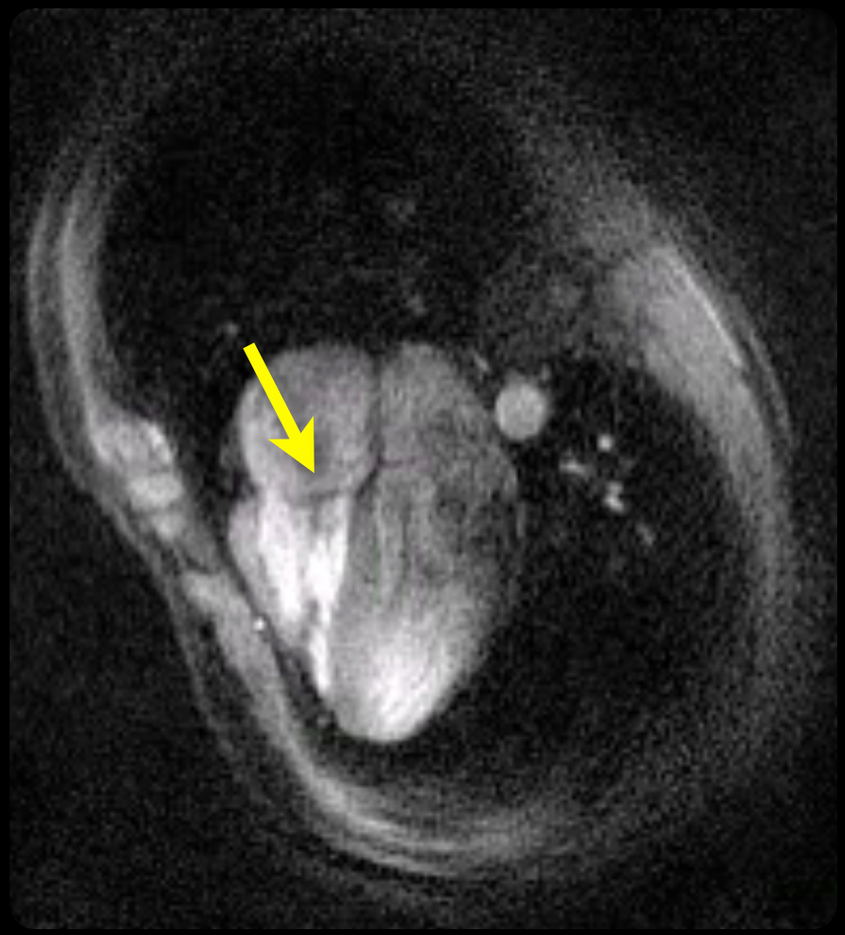

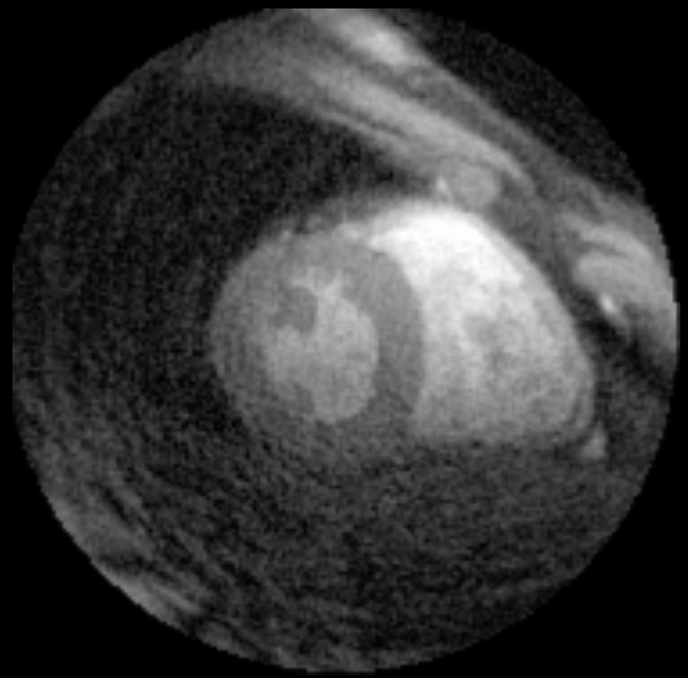

*Courtesy Juan Santos

Flow Imaging Examples

Real-time color flow

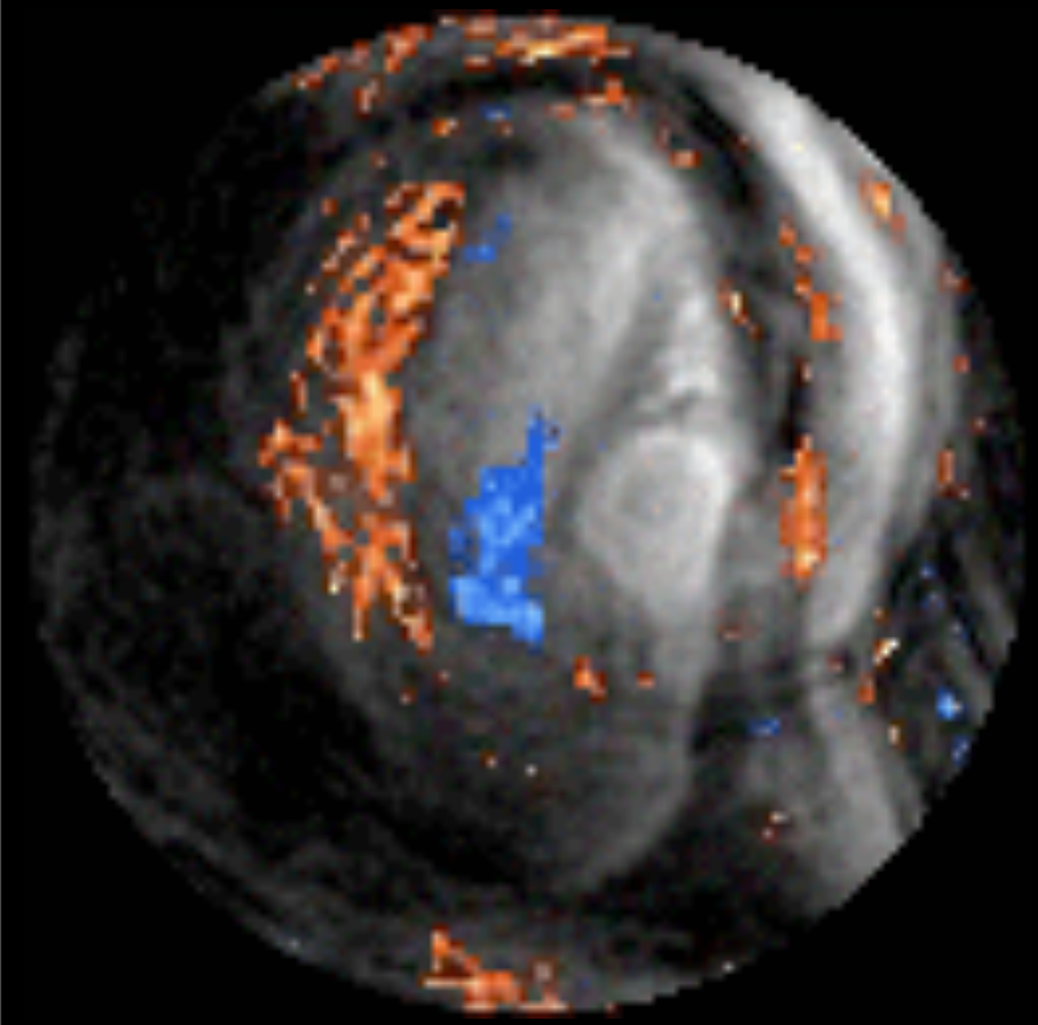

4D flow

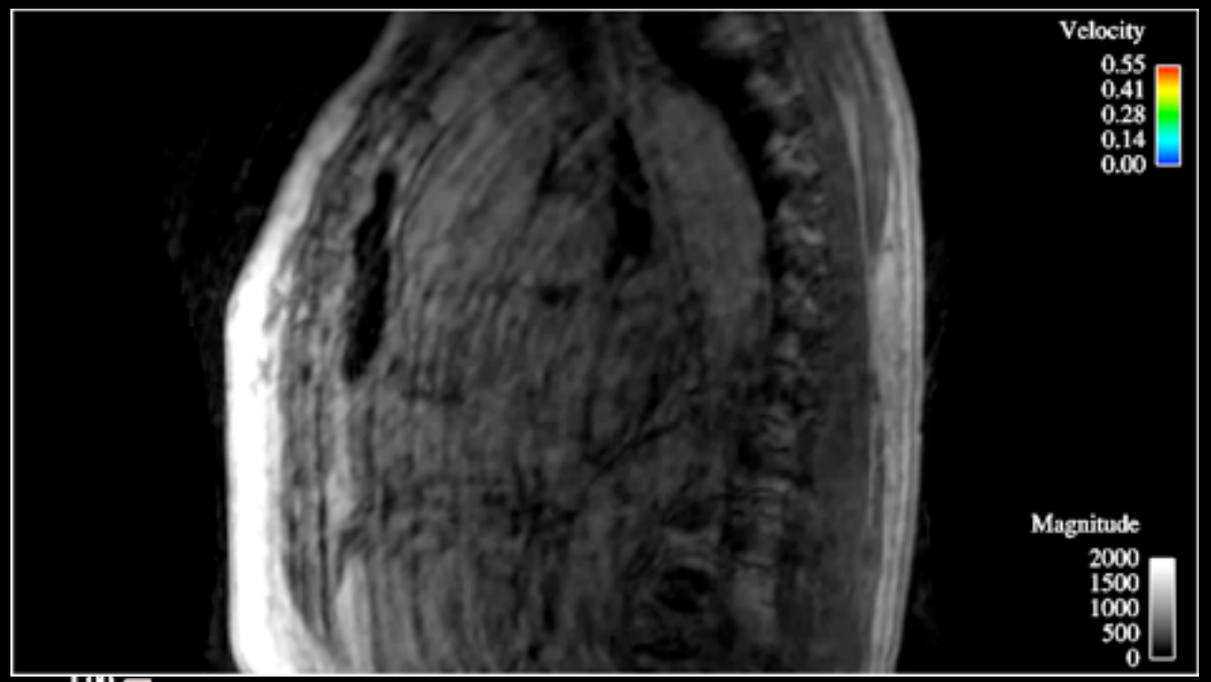

M. Lustig, EECS UC Berkeley

*Juan Santos, Stanford
*Marc Alley, Stanford

Diffusion Examples

T2 weighted standard MRI
3 hours after a stroke

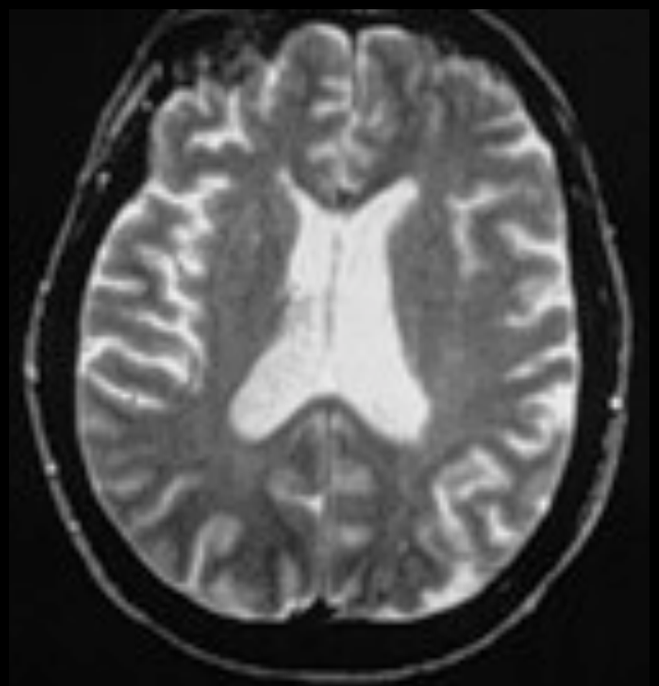

diffusion weighted MRI
3 hours after a stroke

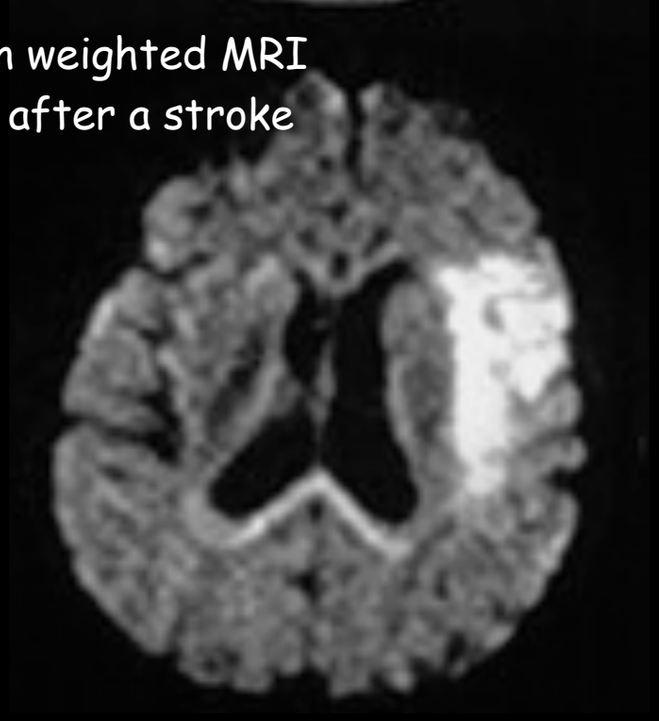

White matter fibers

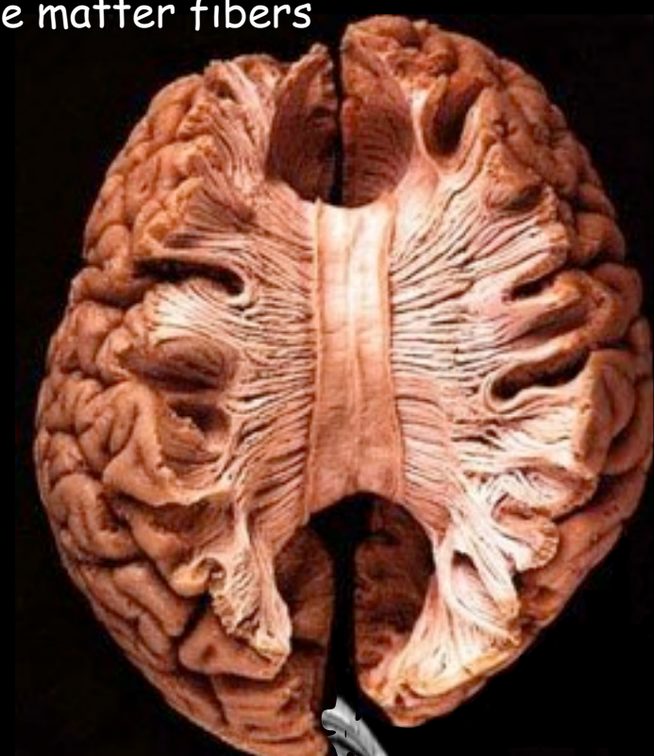

diffusion tensor imaging

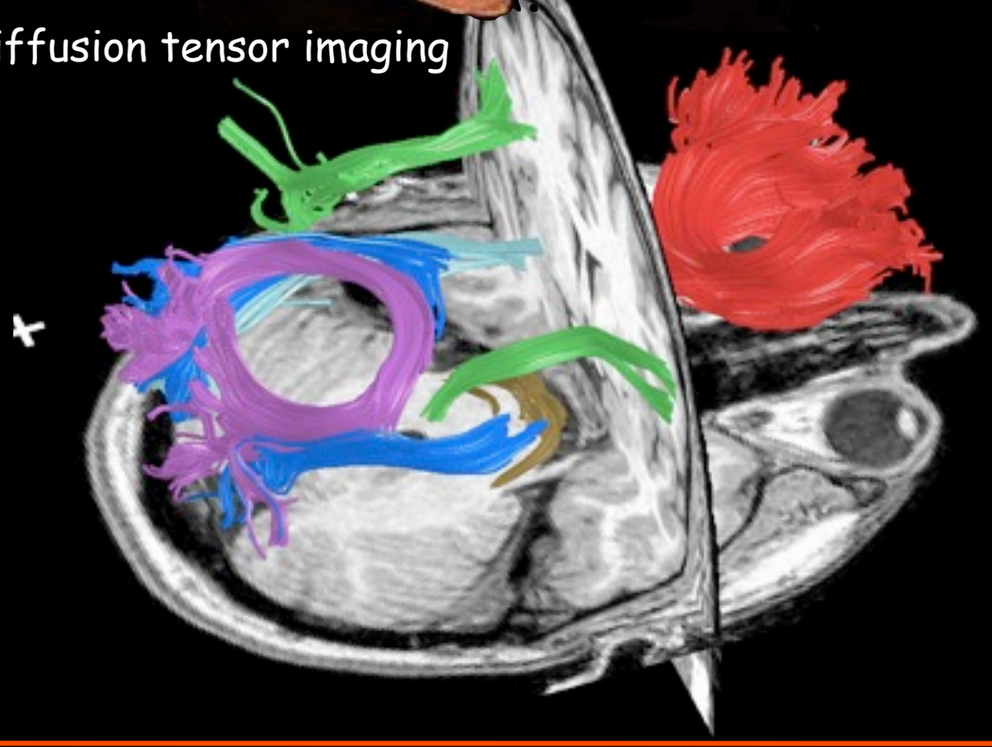

*Dr. Steven Warach, Beth Israel Hospital, Boston, MA
*The Virtual Hospital (www.vh.org); TH Williams, N Gluhbegovic, JY Jew
*Brian Wandell, Stanford

Functional MRI Example

Sensitivity to blood oxygenation - response to brain activity

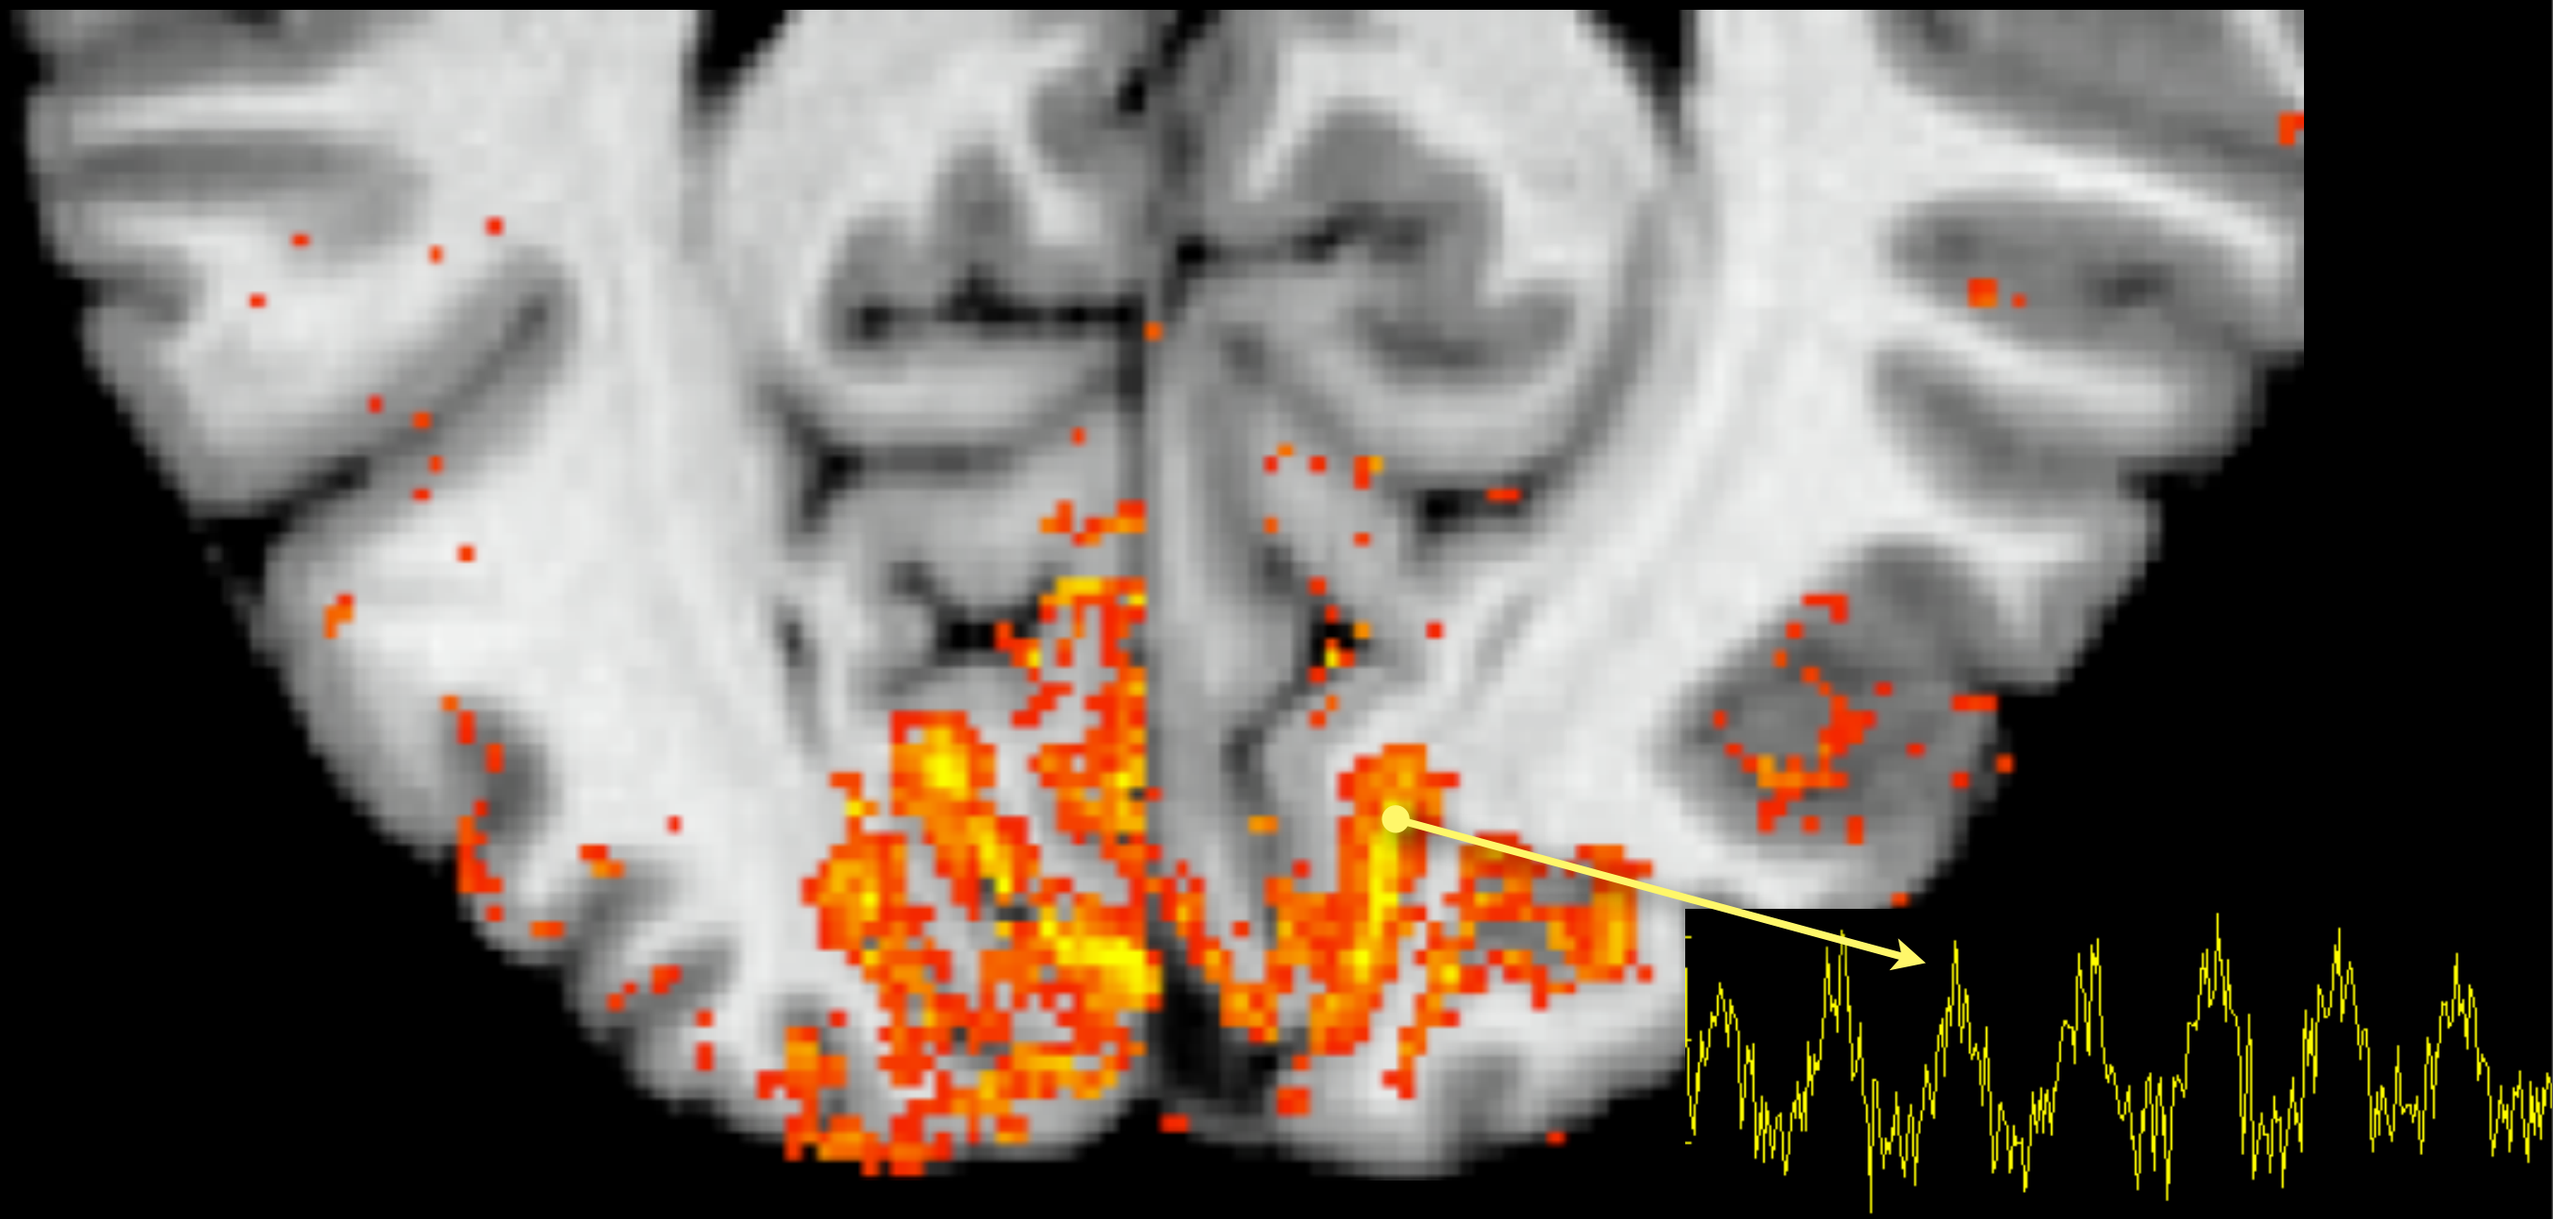

*Karla Miller, Oxford
*Brian Wandell, Stanford

Taking fMRI further

- fMRI decoding : "Mind Reading"
  Gallant Lab, UC Berkeley

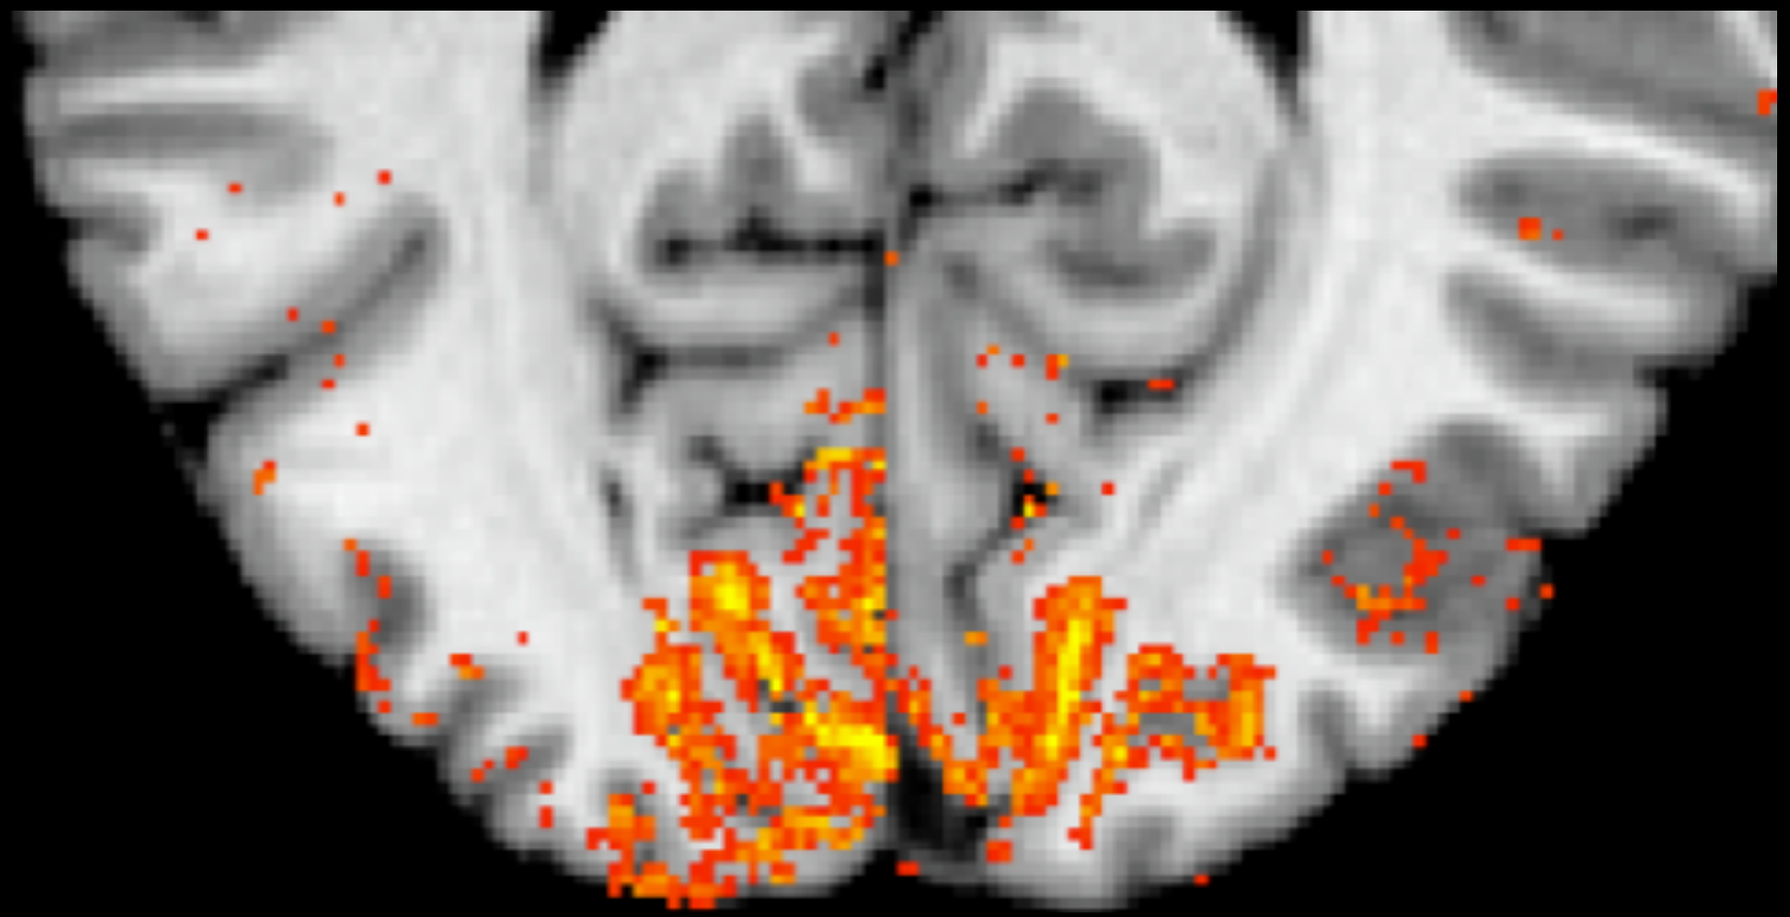

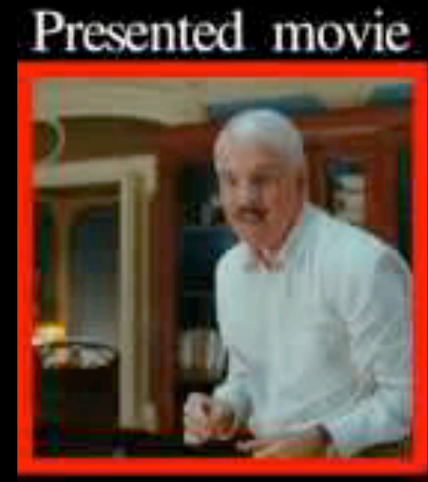

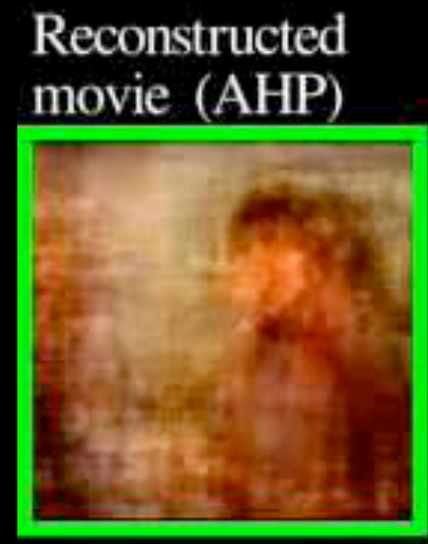

Spectroscopy Imaging

- Functional Imaging (metabolism)
- Also other nuclei (13C, phosphor)

* Daniel Vigneron and Simon Hu, UCSF

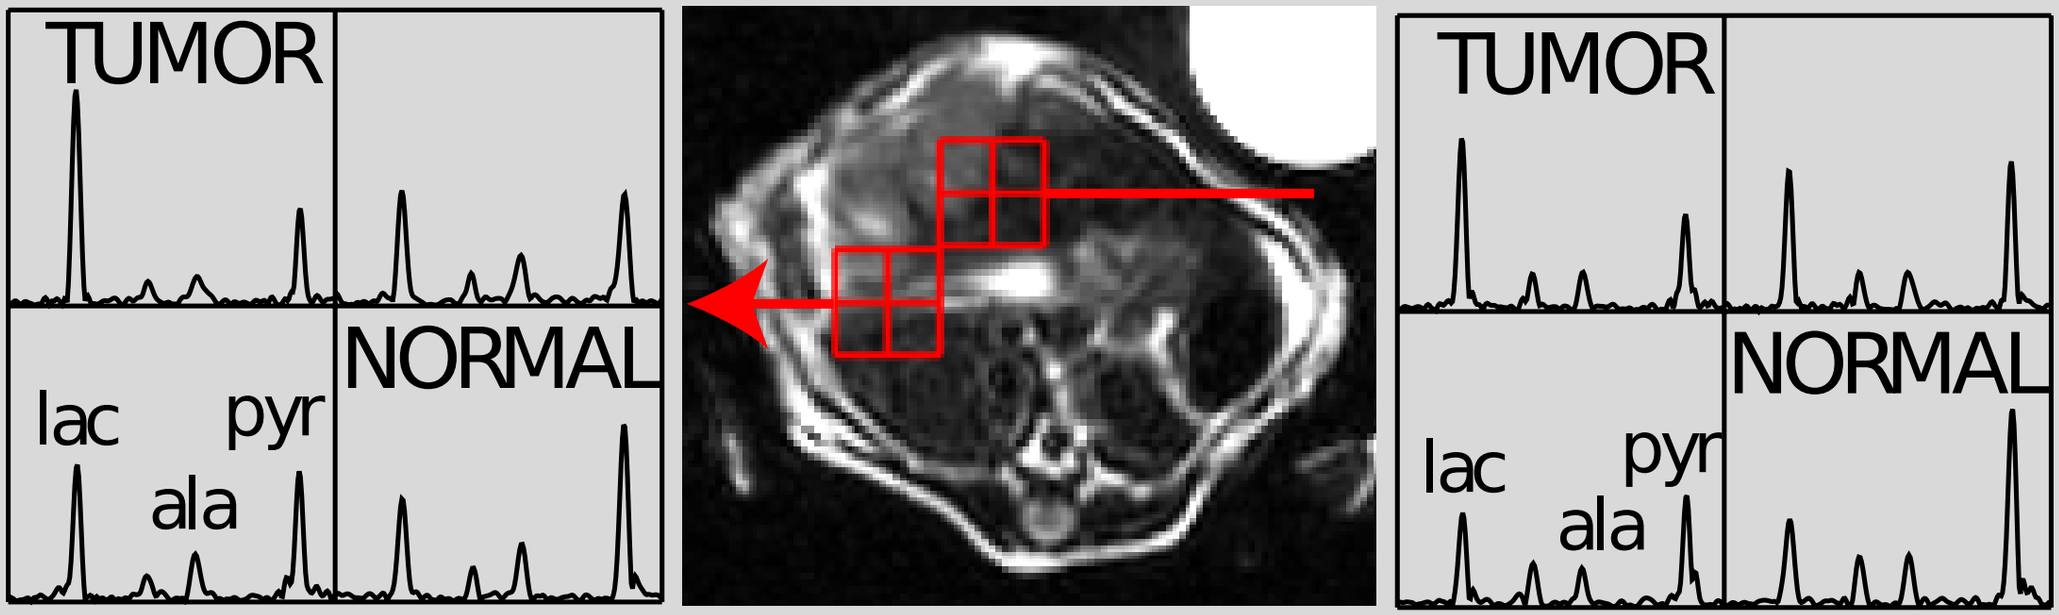

Phase

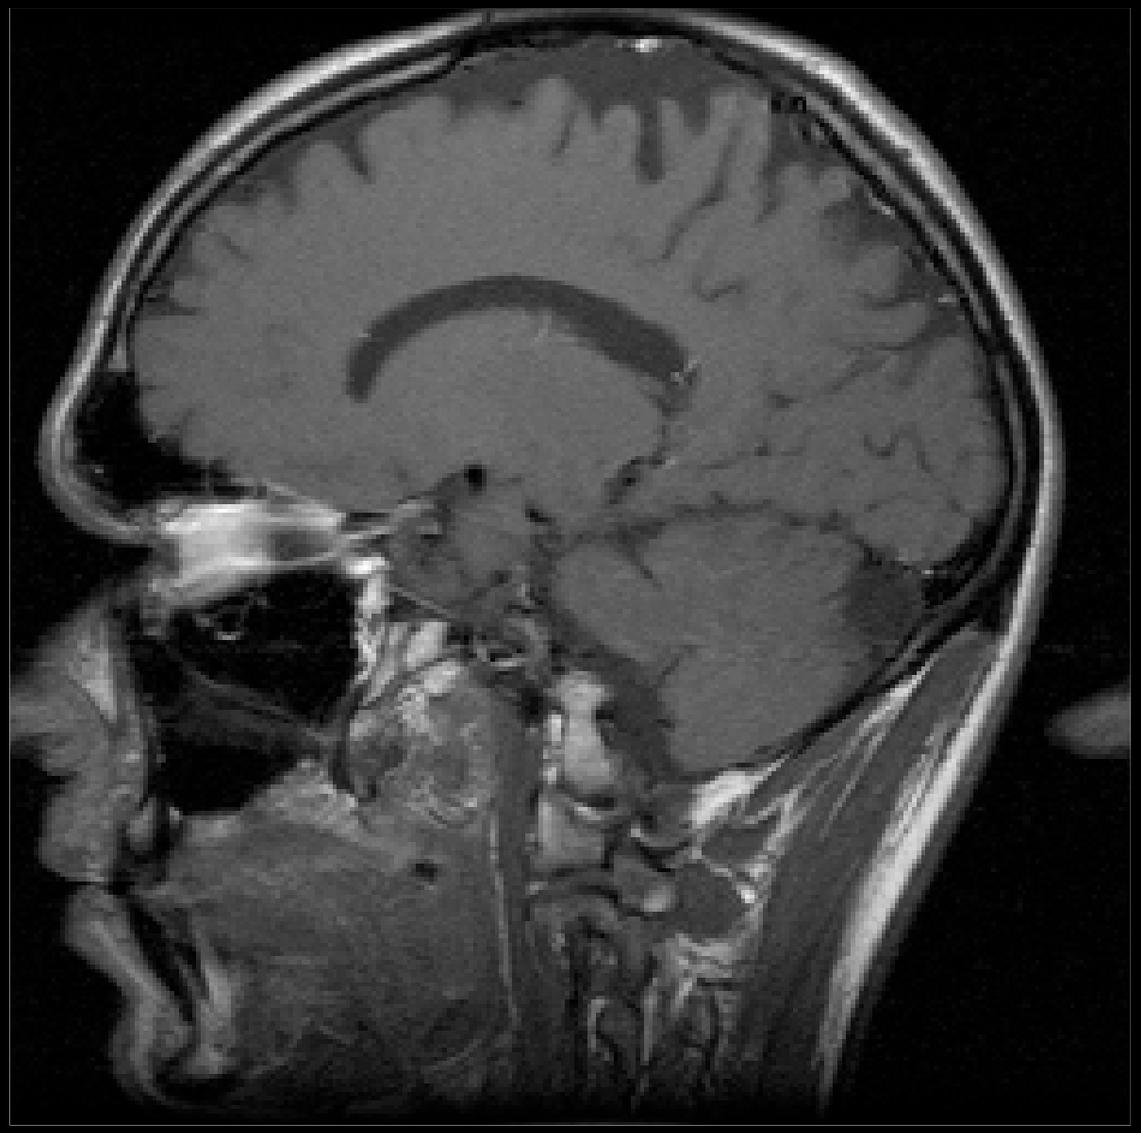

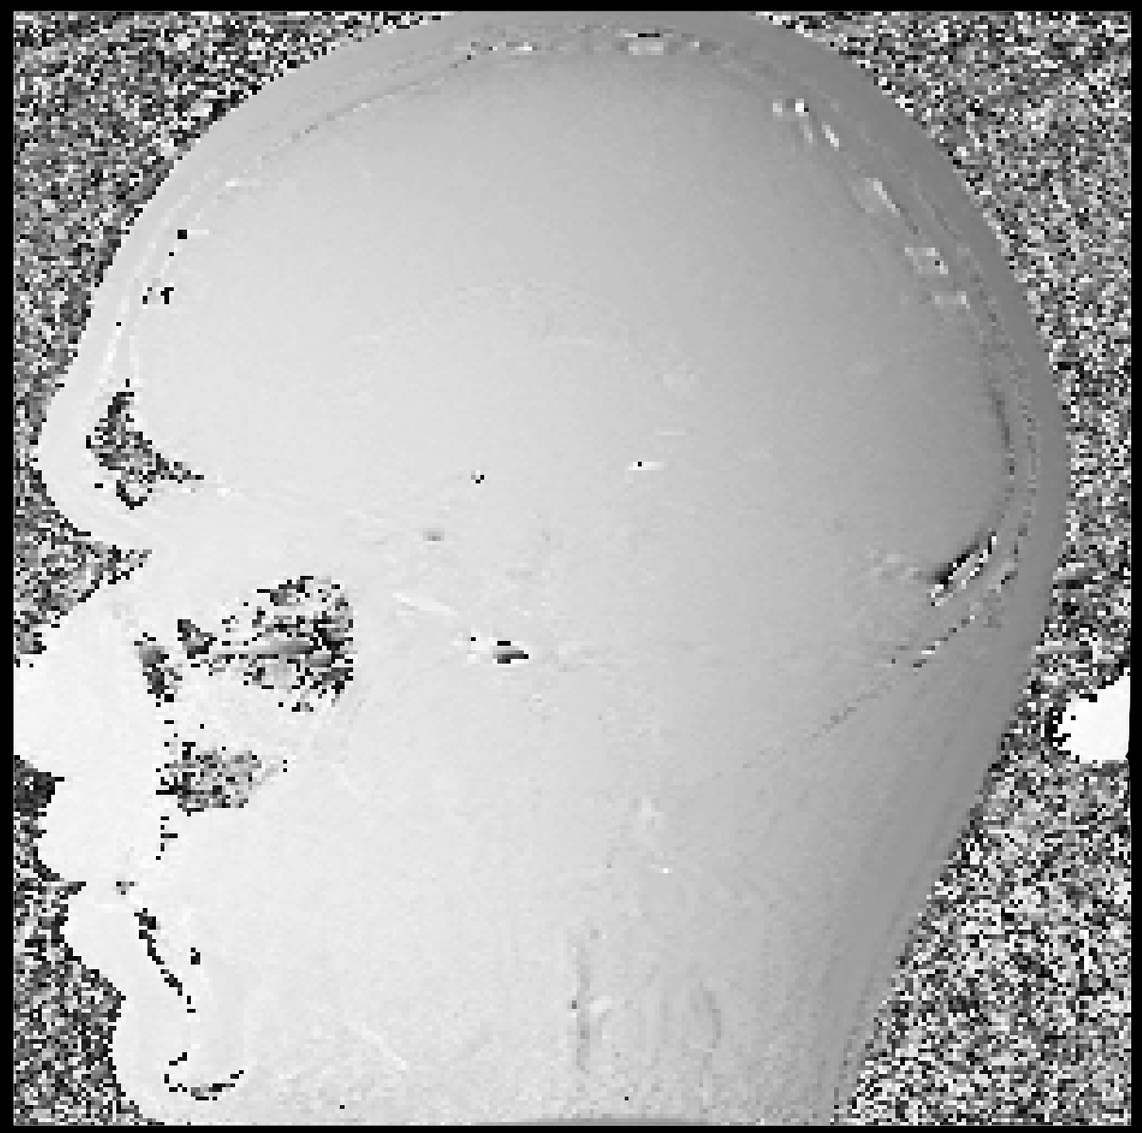

*K. Pauly, G. Gold, RAD220

Breast

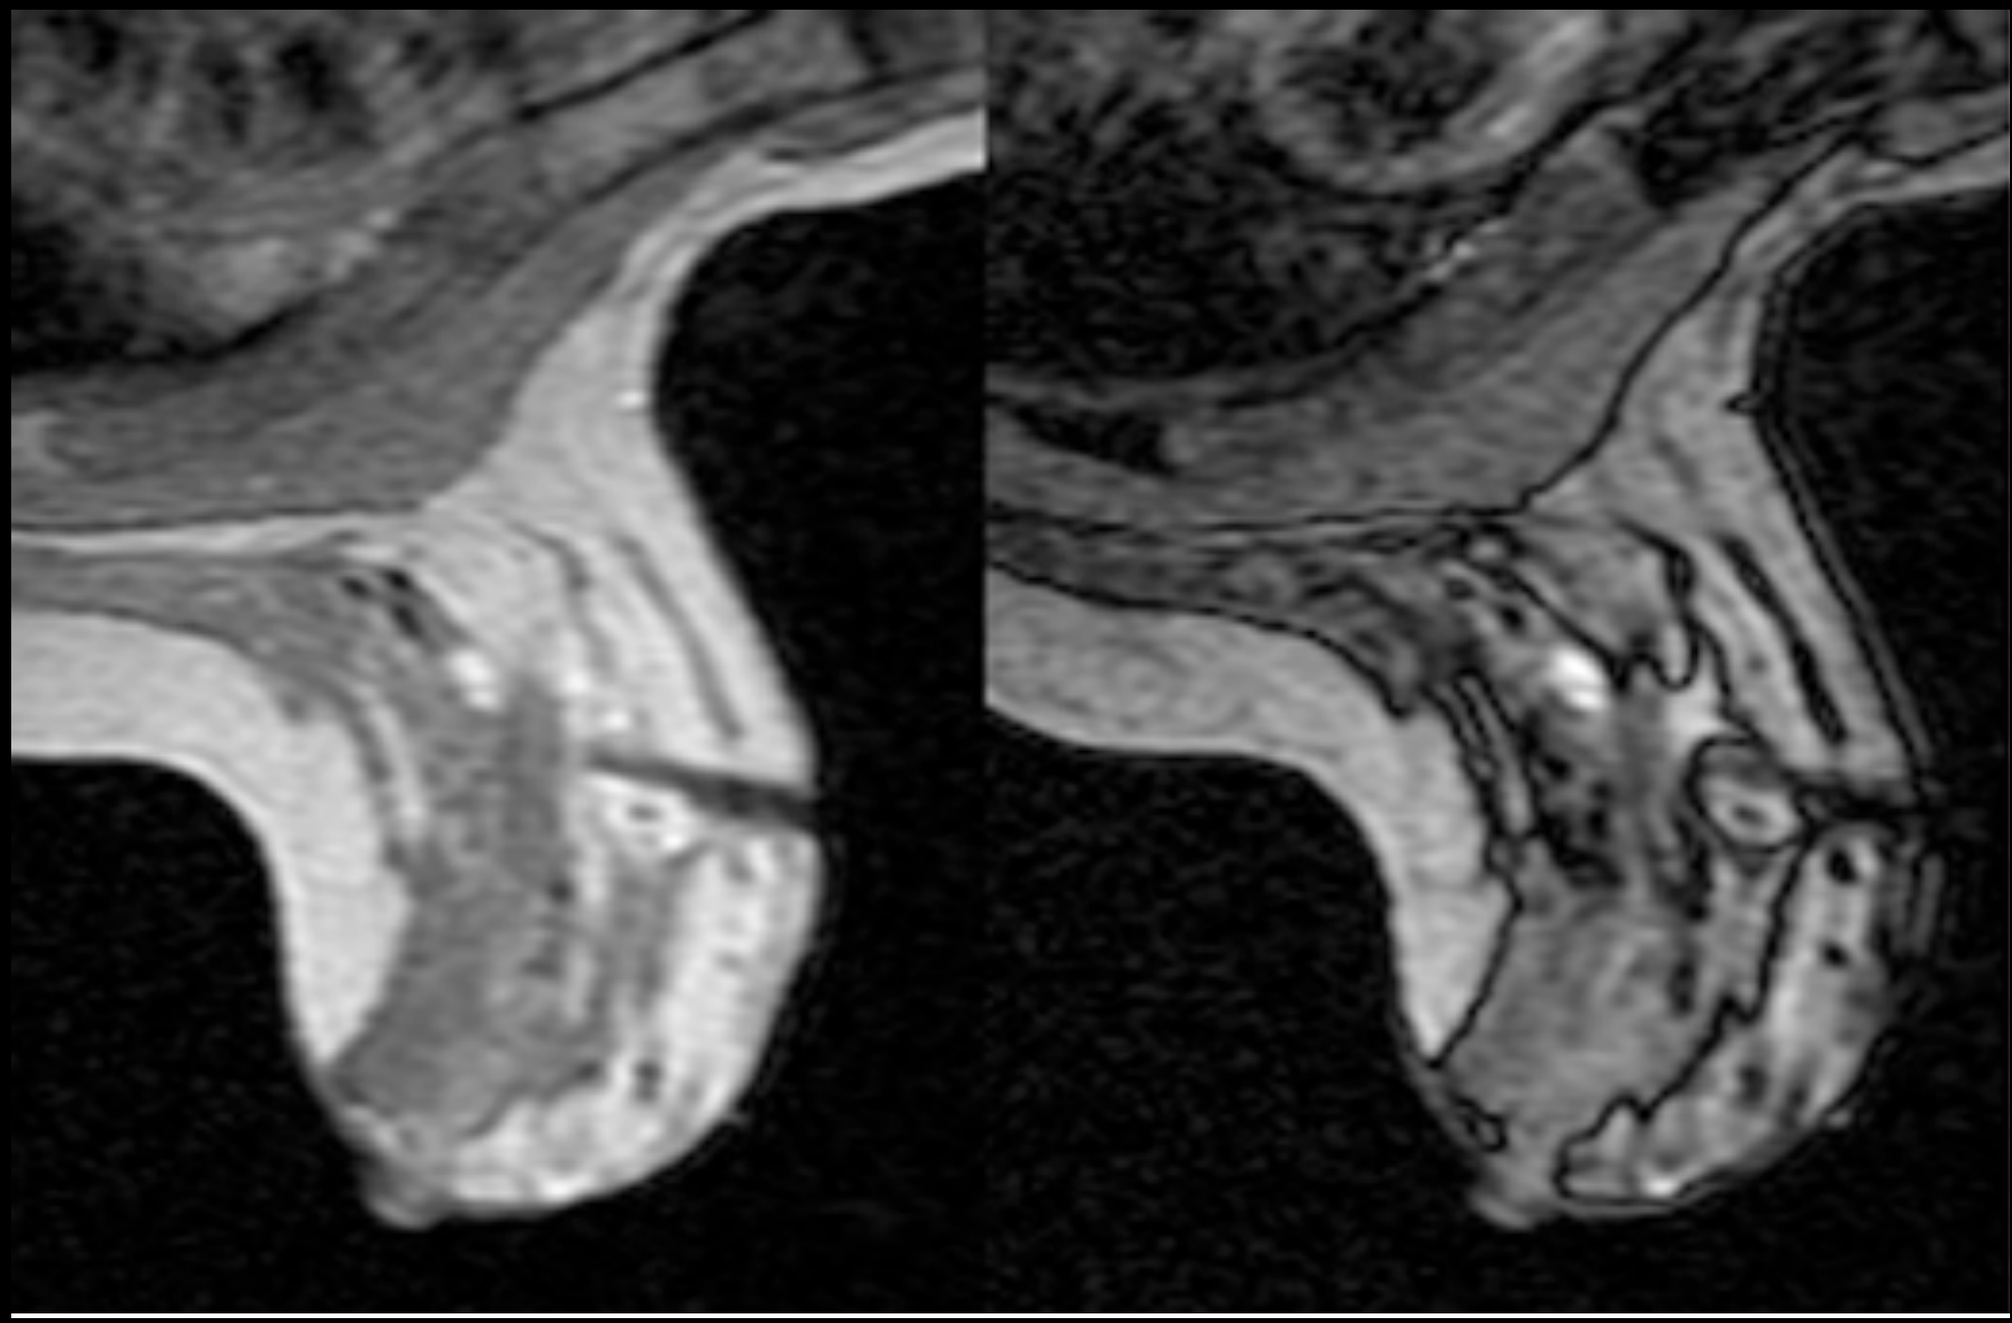

*K. Pauly, G. Gold, RAD220

Spin-Echo vs Gradient Echo

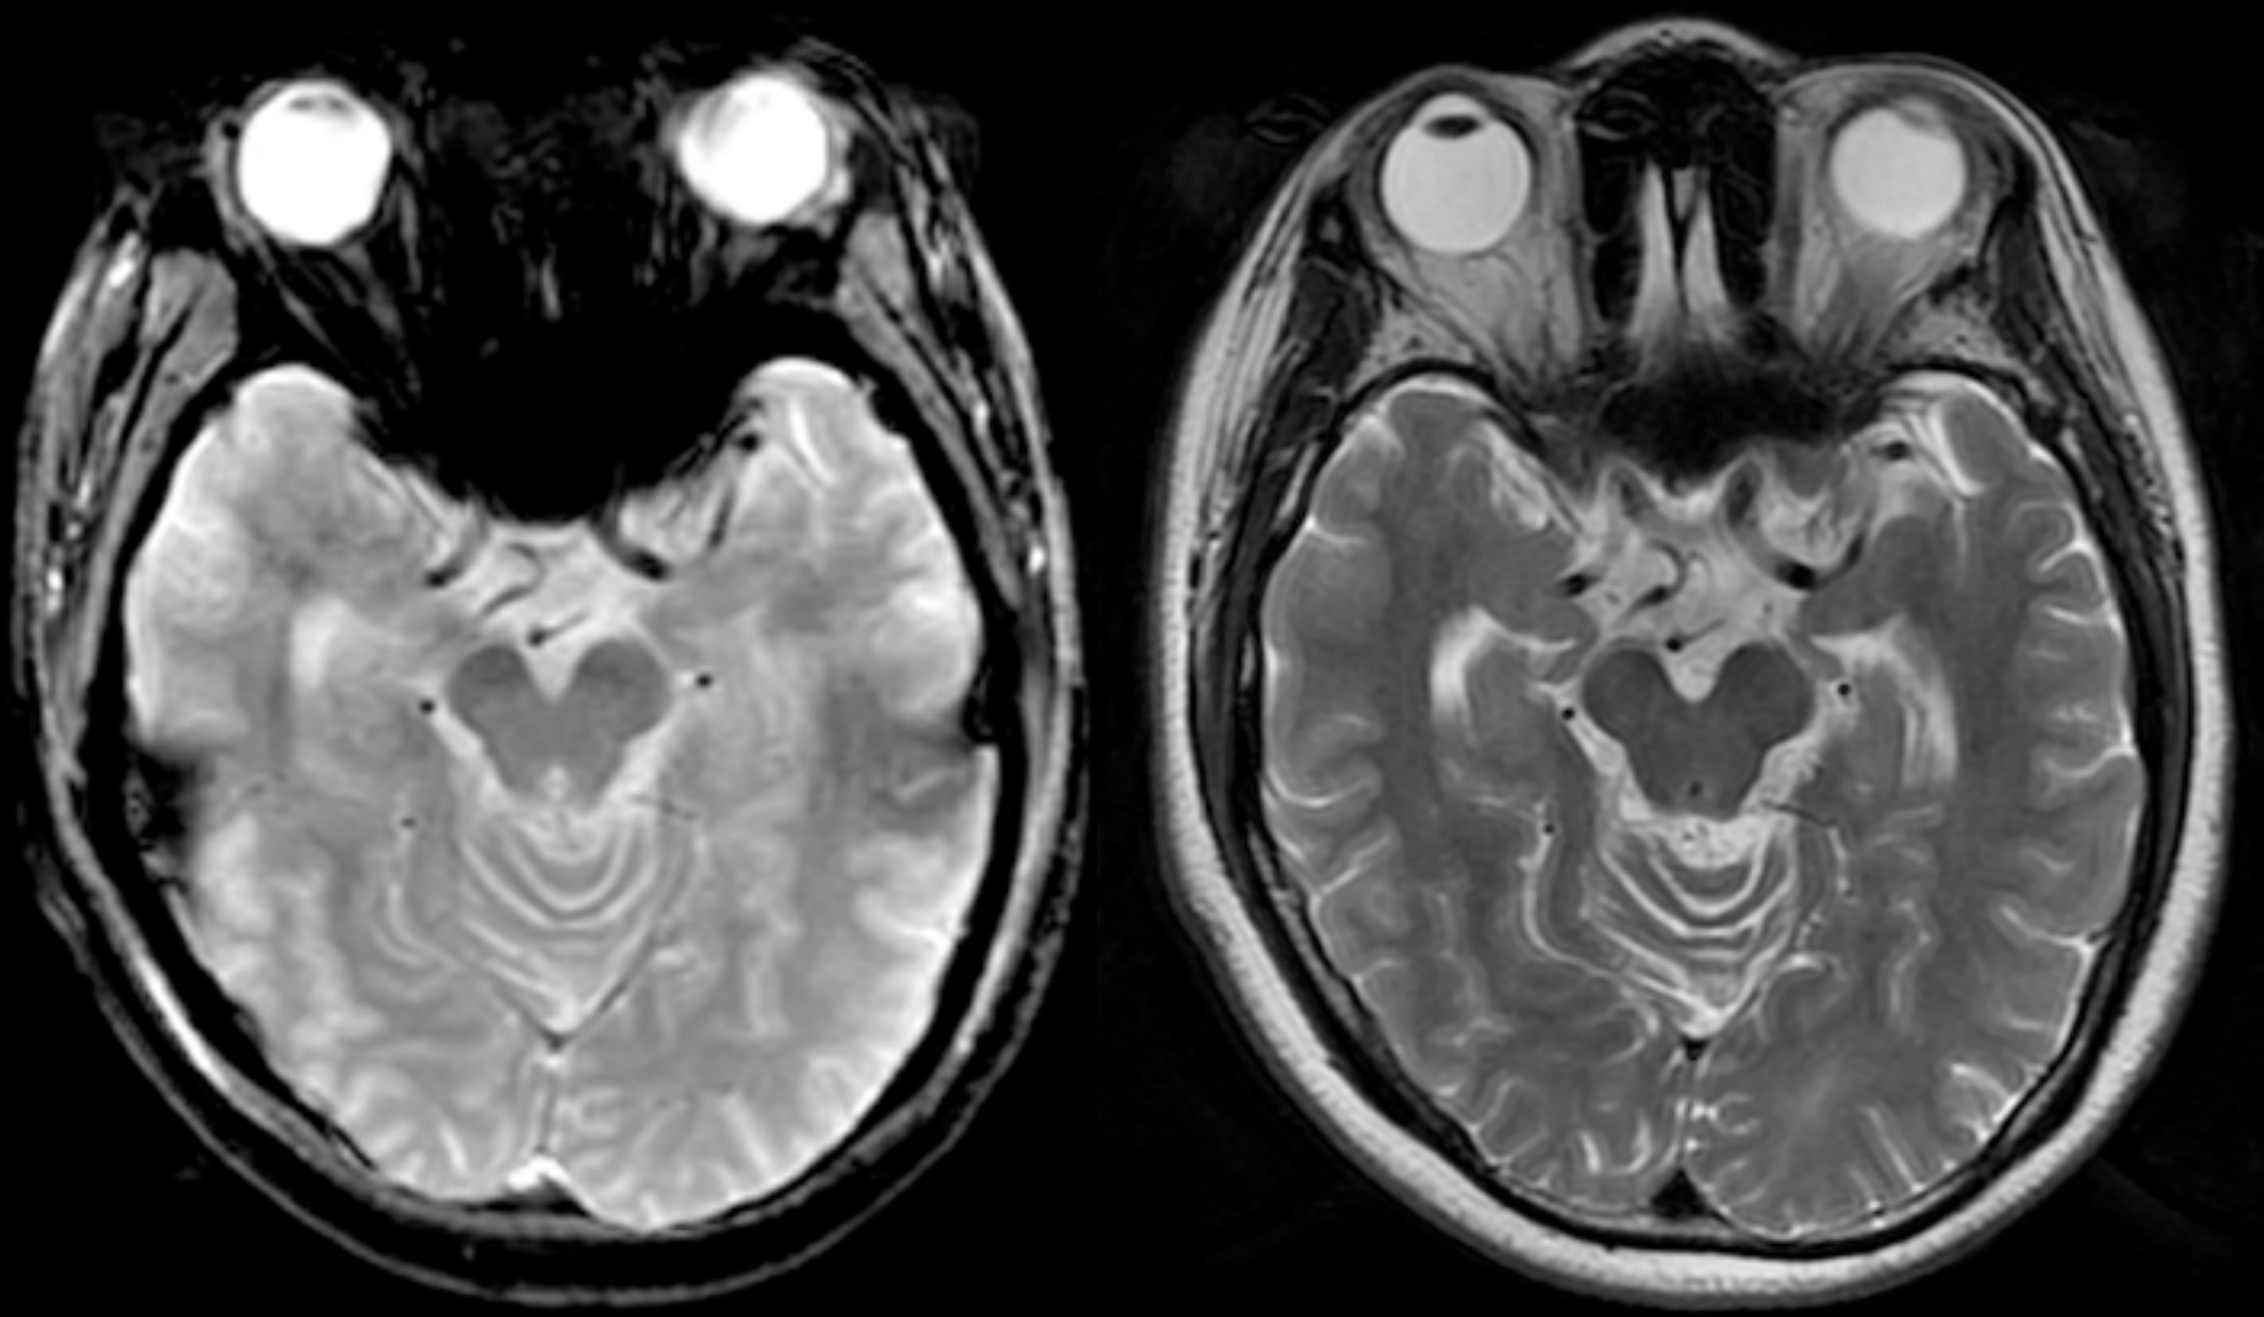

*K. Pauly, G. Gold, RAD220

Chemical-shift

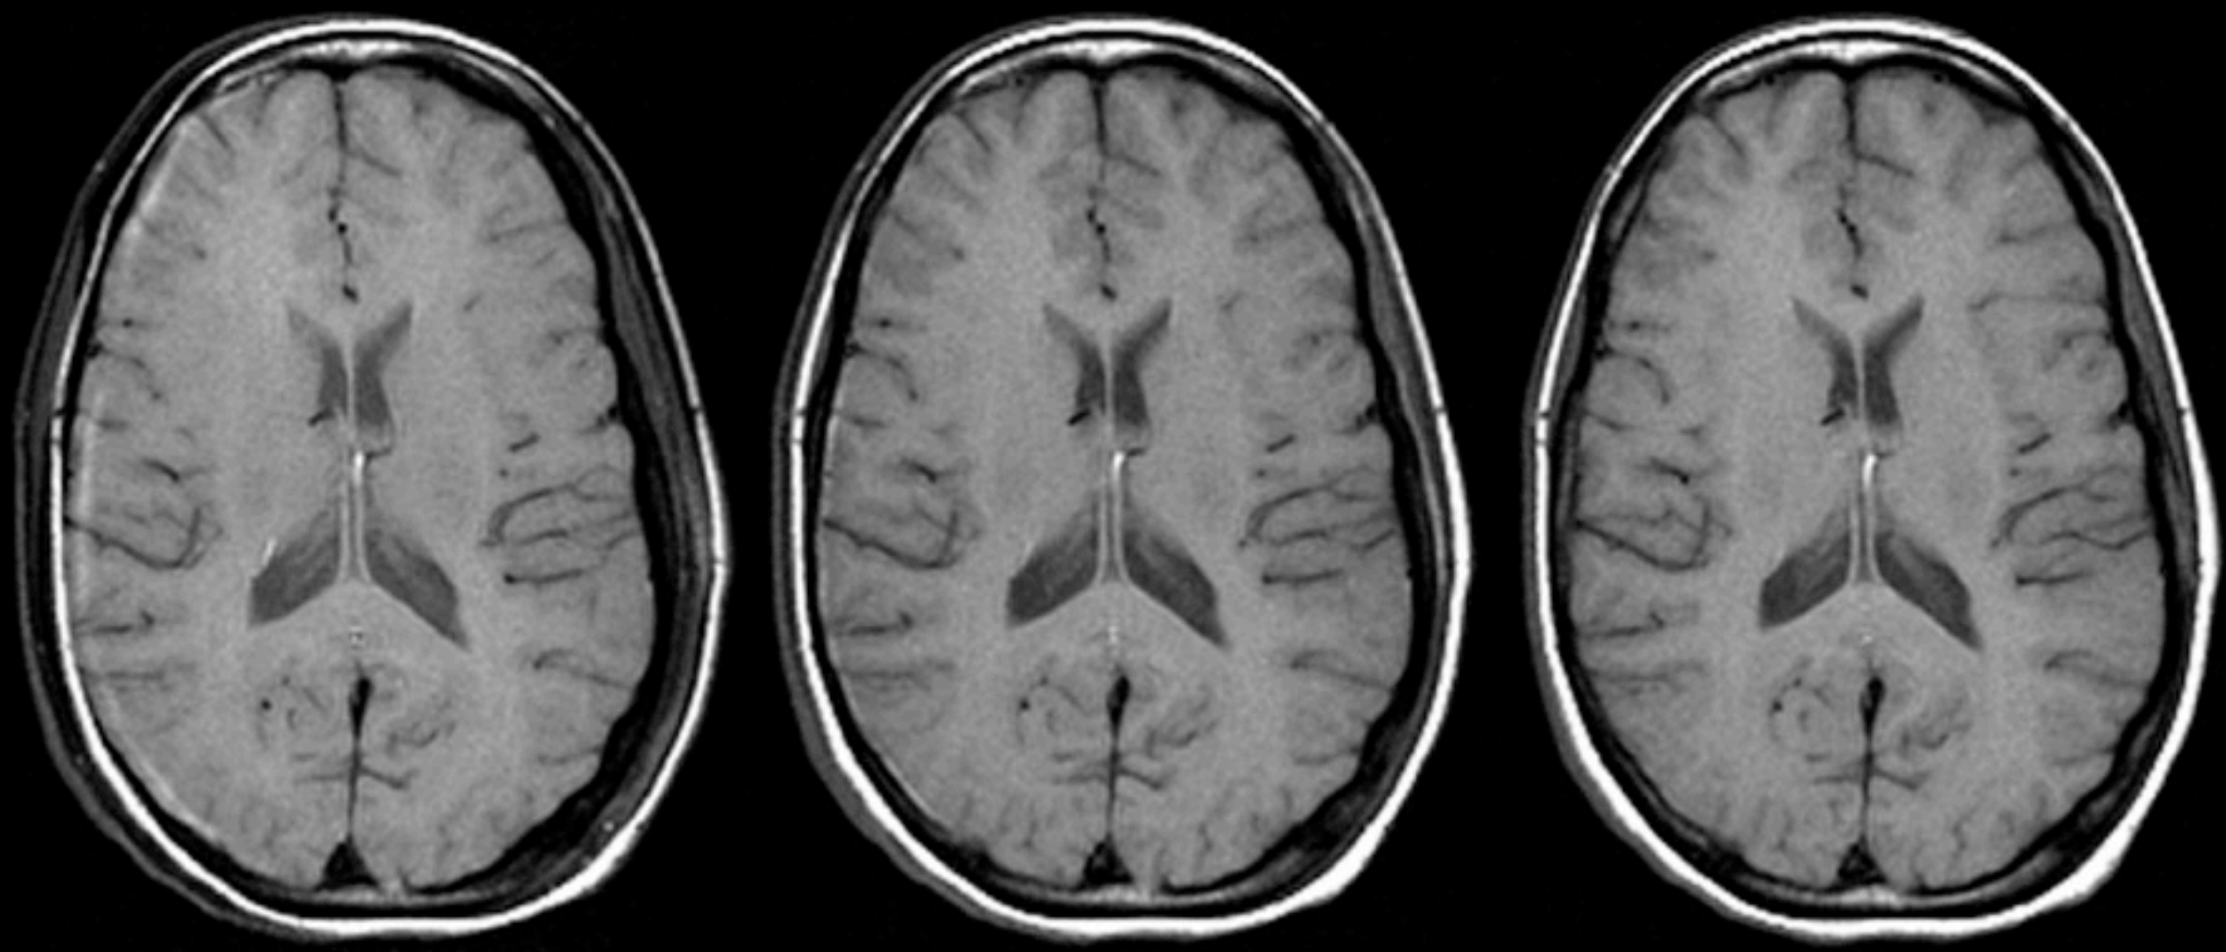

*images, courtesy of Brian Hargreaves

Metal Artifacts

*images, courtesy of Brian Hargreaves

Motion Artifacts

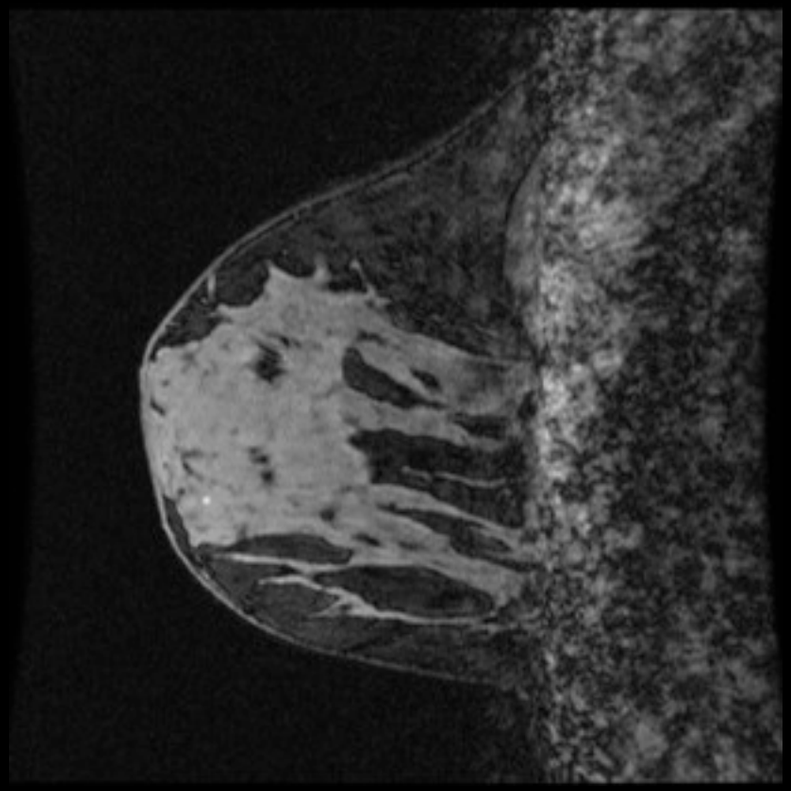

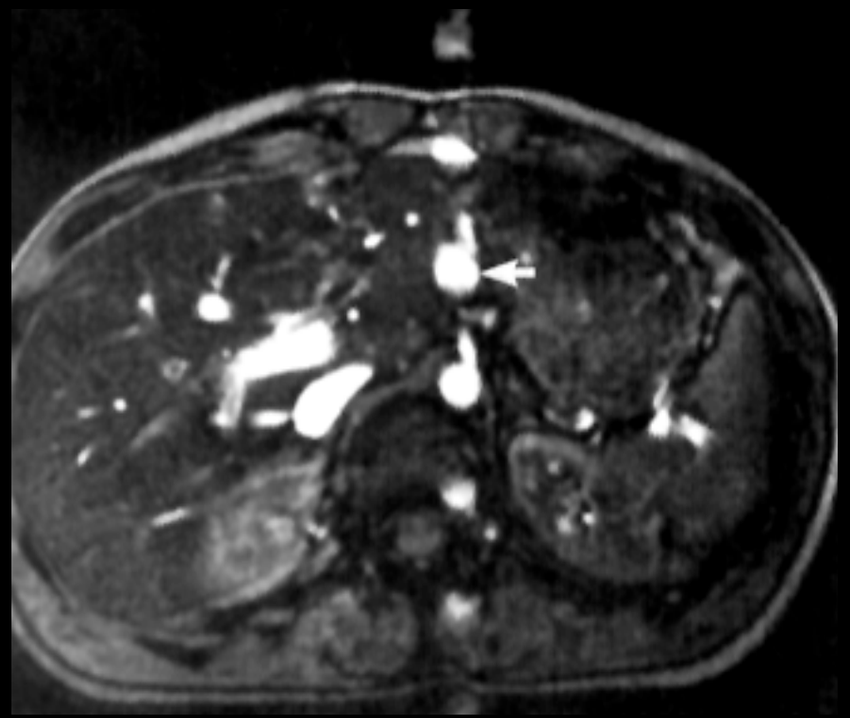

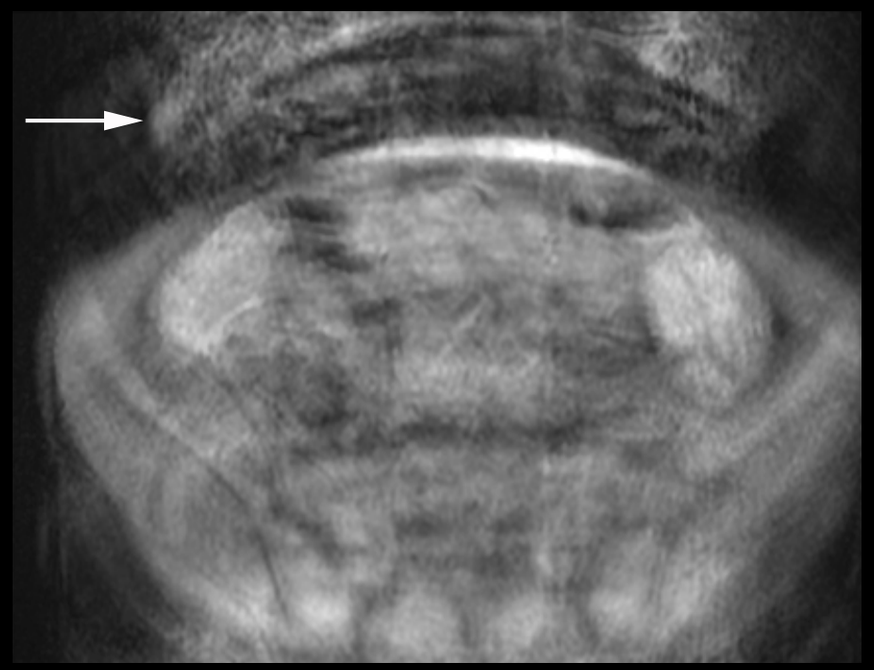

How Does MRI Work?

- Magnetic Polarization
  -- Very strong uniform magnet
- Excitation
  -- Very powerful RF transmitter
- Acquisition
  -- Location is encoded by gradient magnetic fields
  -- Very powerful audio amps

Polarization

- Protons have a magnetic moment
- Protons have spins
- Like rotating magnets

Polarization

- Body has a lot of protons
- In a strong magnetic field B0, spins align with B0 giving a net magnetization

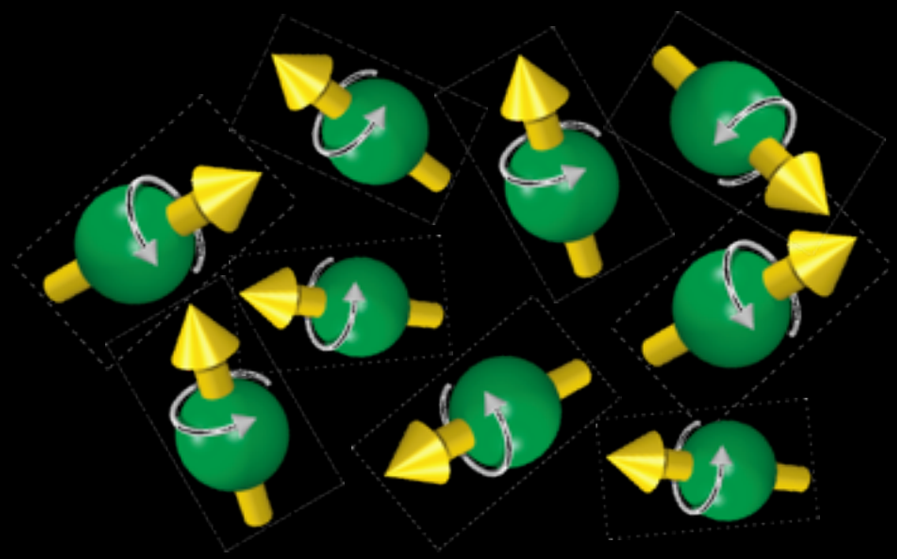

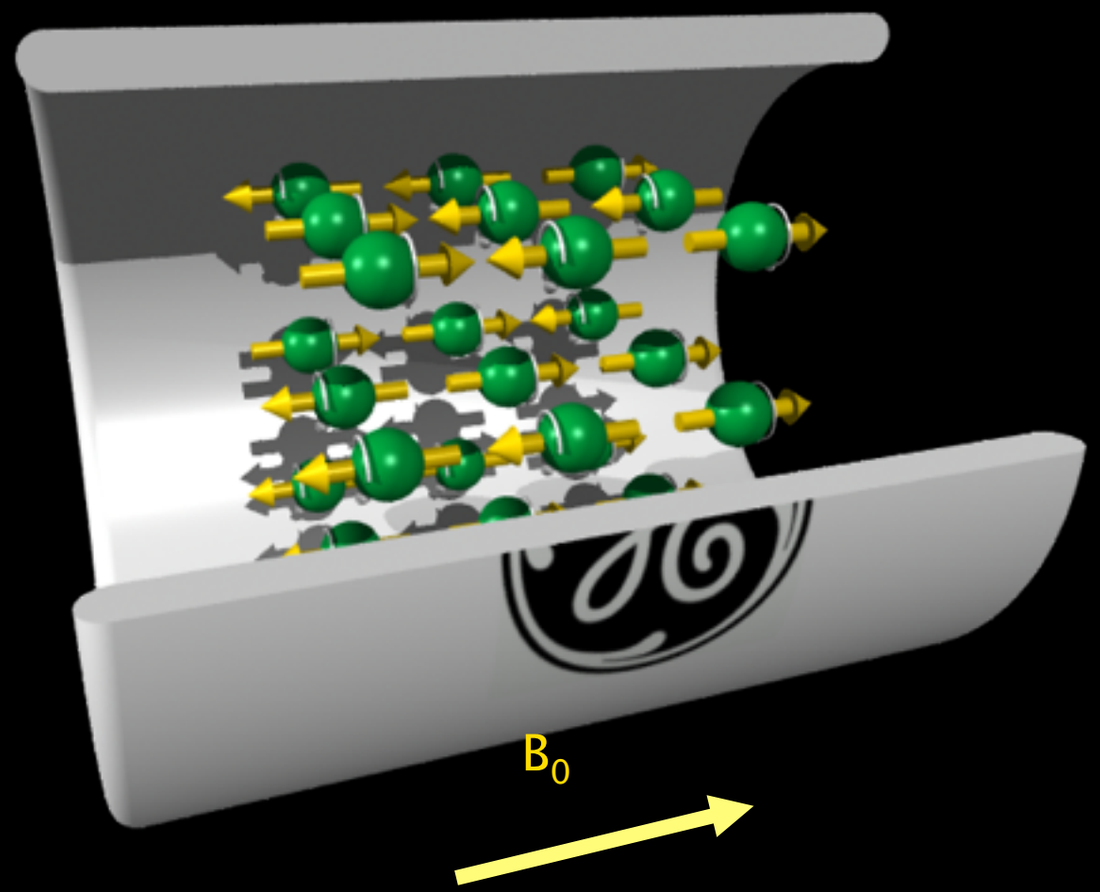

*Graphic rendering Bill Overall

Polarizing Magnet

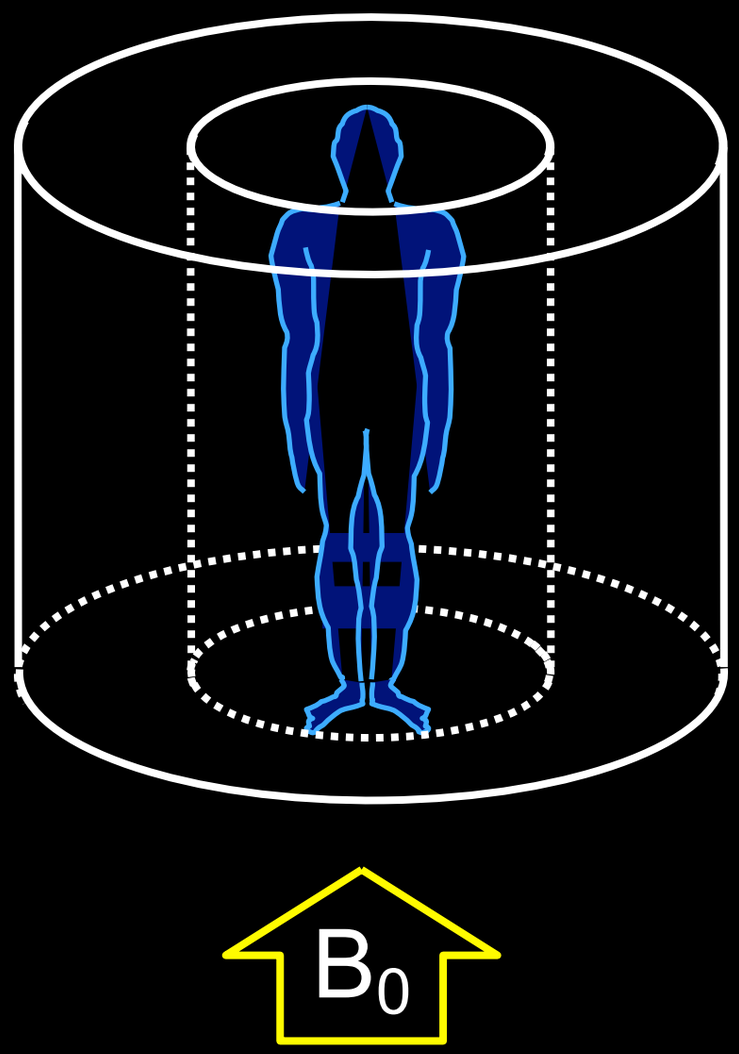

- 0.1 to 12 Tesla
- 0.5 to 3 T common
- 1 T is 10,000 Gauss
- Earth's field is 0.5G
- Typically a superconducting magnet

Typical 1.5T MRI System

Polarizaion

- Polarization results in net magnetization

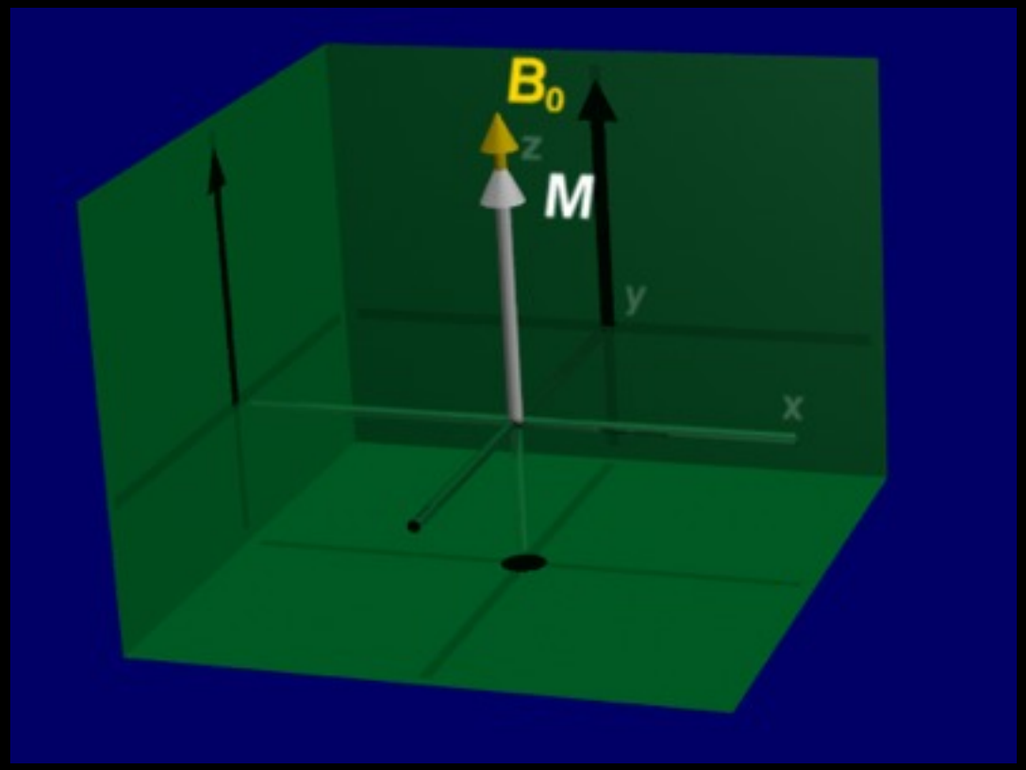

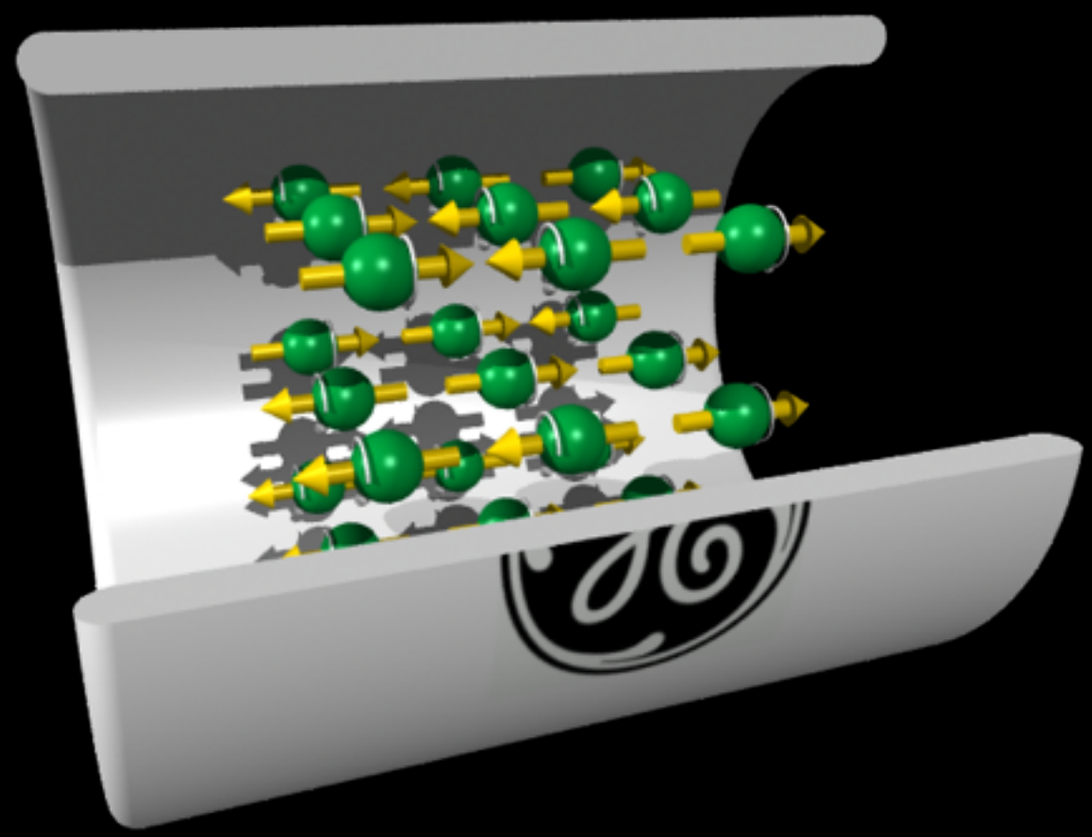

Free Precession

- Much like a spinning top
- Frequency proportional to the field
- f = 64MhZ @ 1.5T

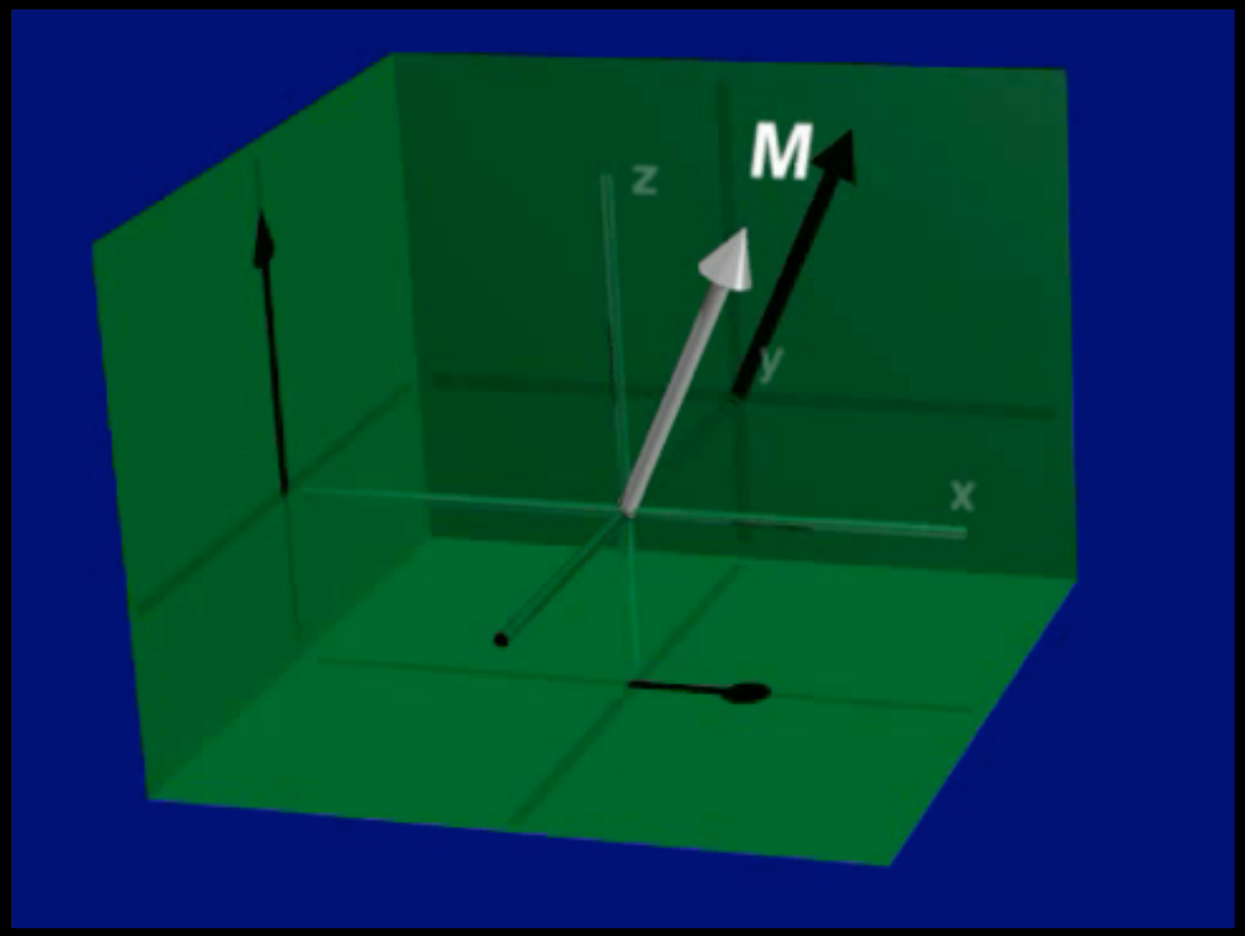

MIT physics demos

Free Precession

- Precession induces magnetic flux
- Flux induces voltage in a coil

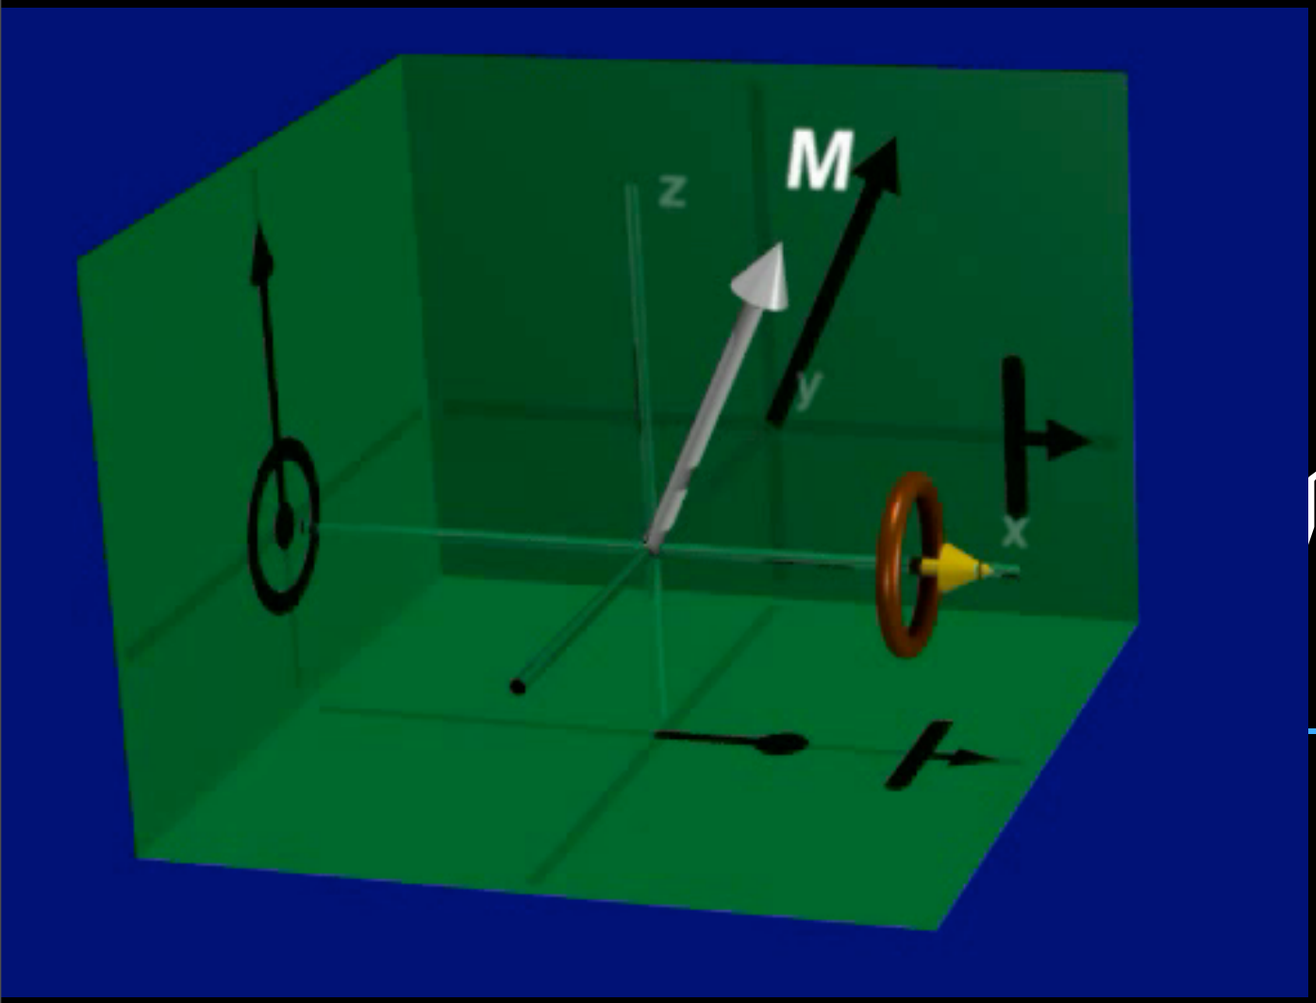

Signal

Intro to MRI - The NMR signal

- Signal from ^1H (mostly water)
- Magnetic field ⇒ Magnetization
- Radio frequency ⇒ Excitation
- Frequency ∝ Magnetic field

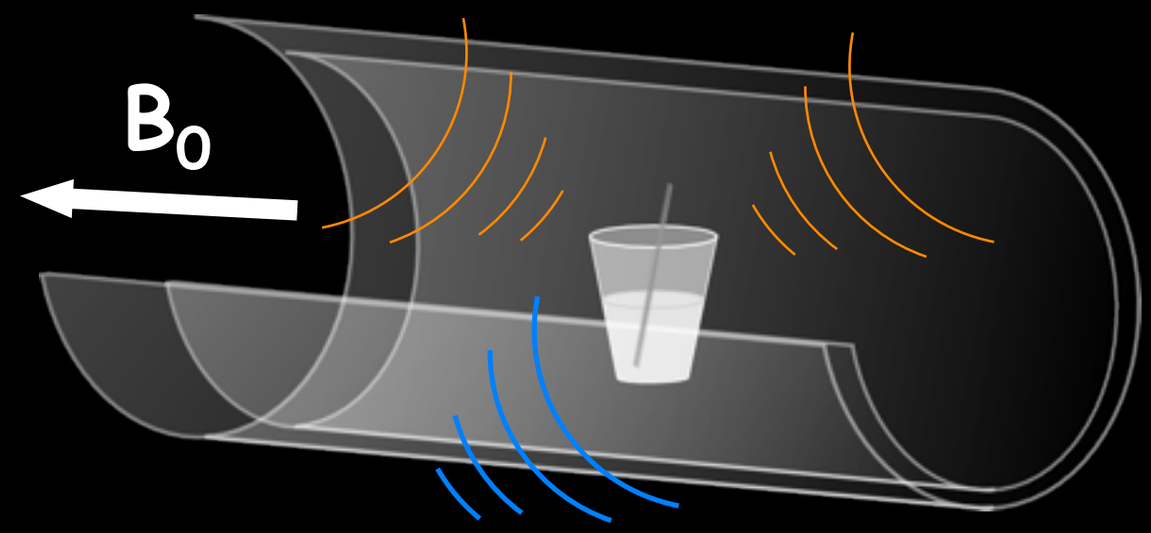

time

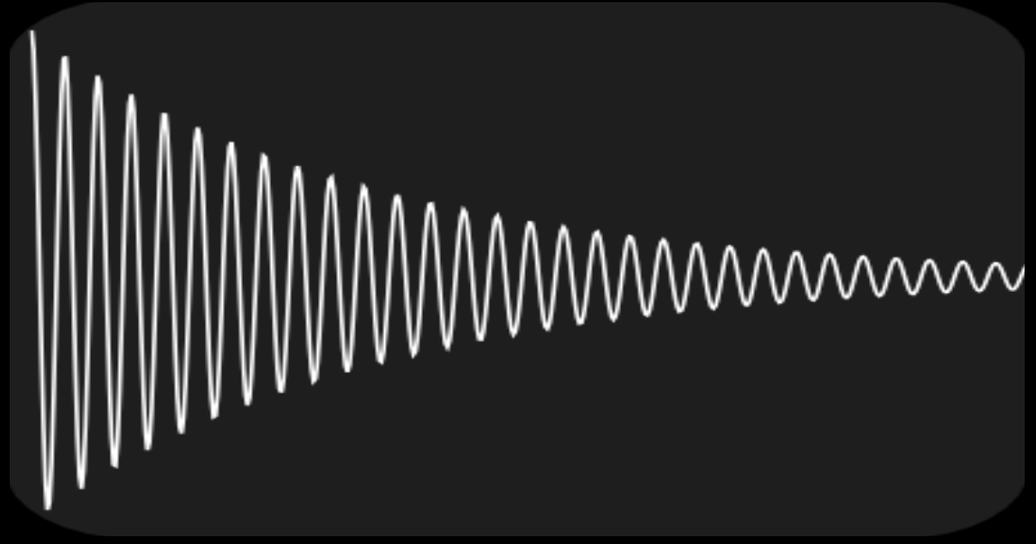

frequency

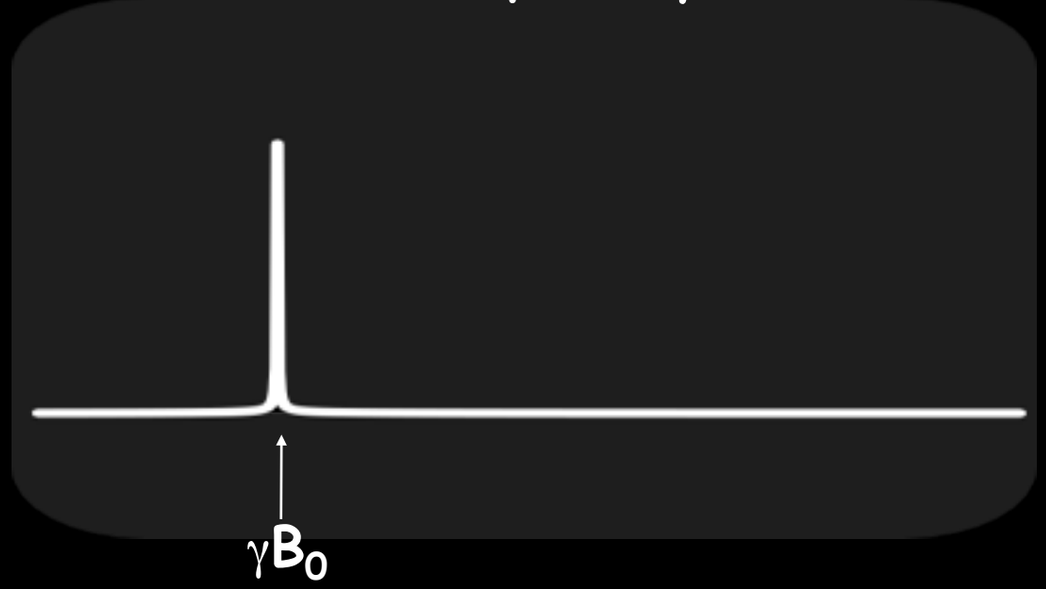

Intro to MRI - The NMR signal

- Signal from ^1H (mostly water)
- Magnetic field ⇒ Magnetization
- Radio frequency ⇒ Excitation
- Frequency ∝ Magnetic field

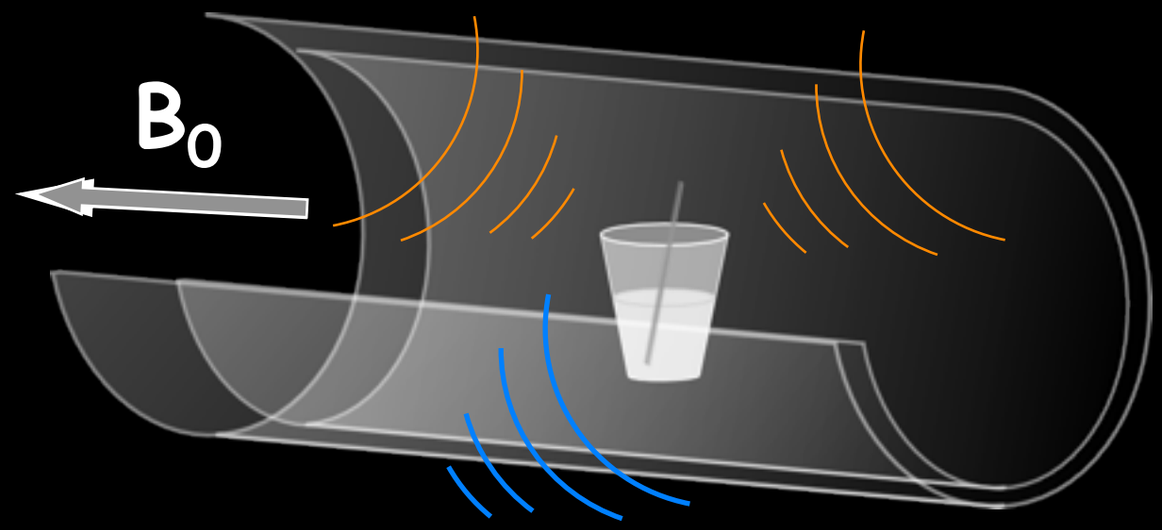

time

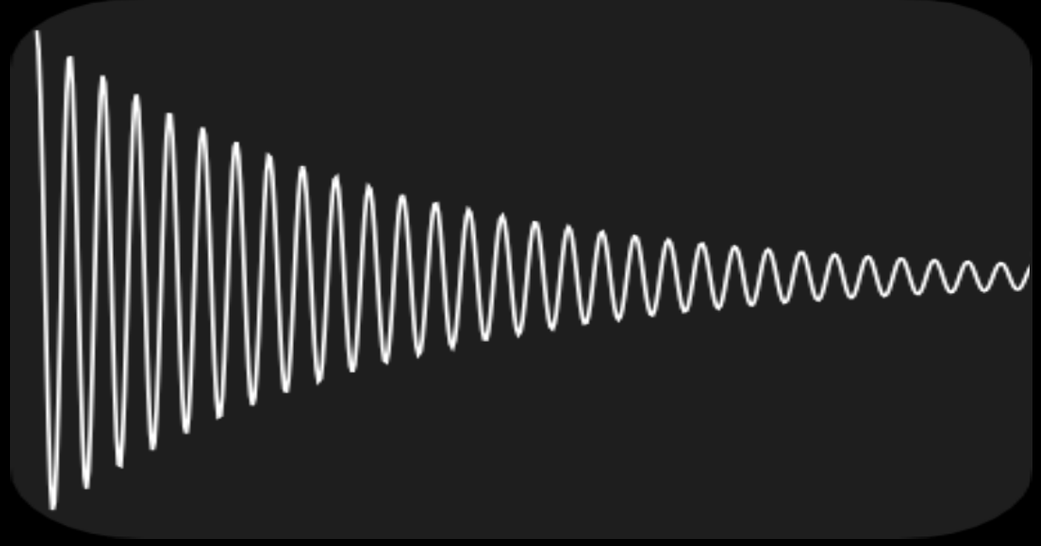

frequency

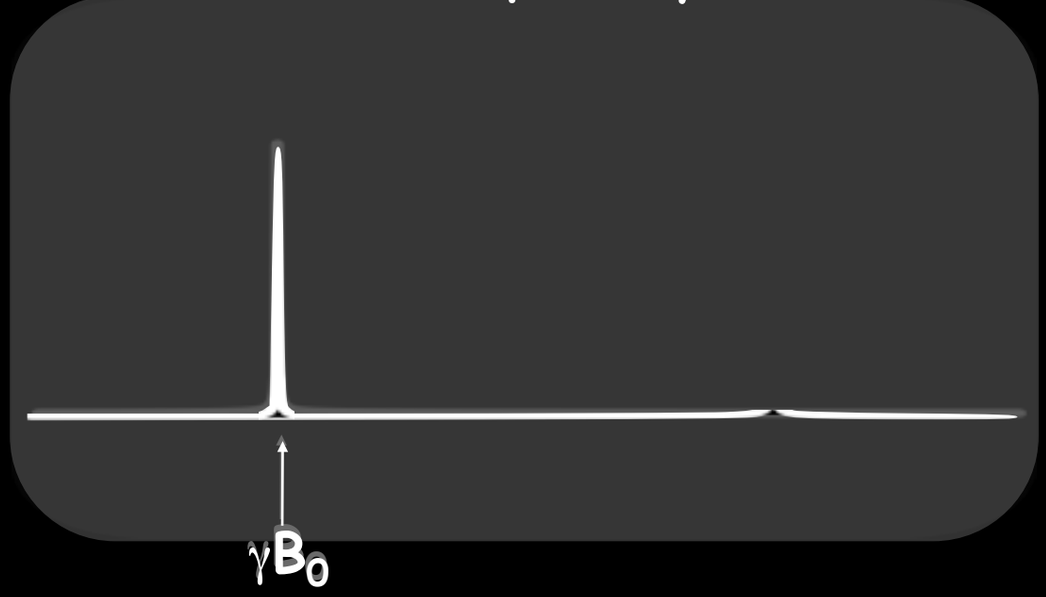

Intro to MRI - Imaging

- B_0 Missing spatial information

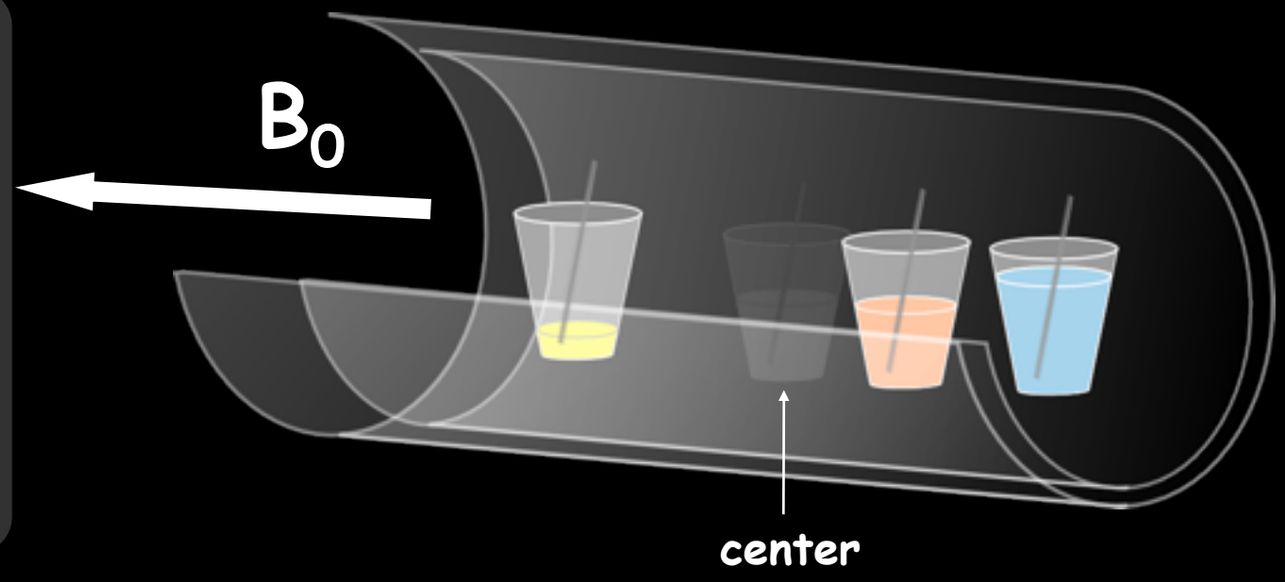

time

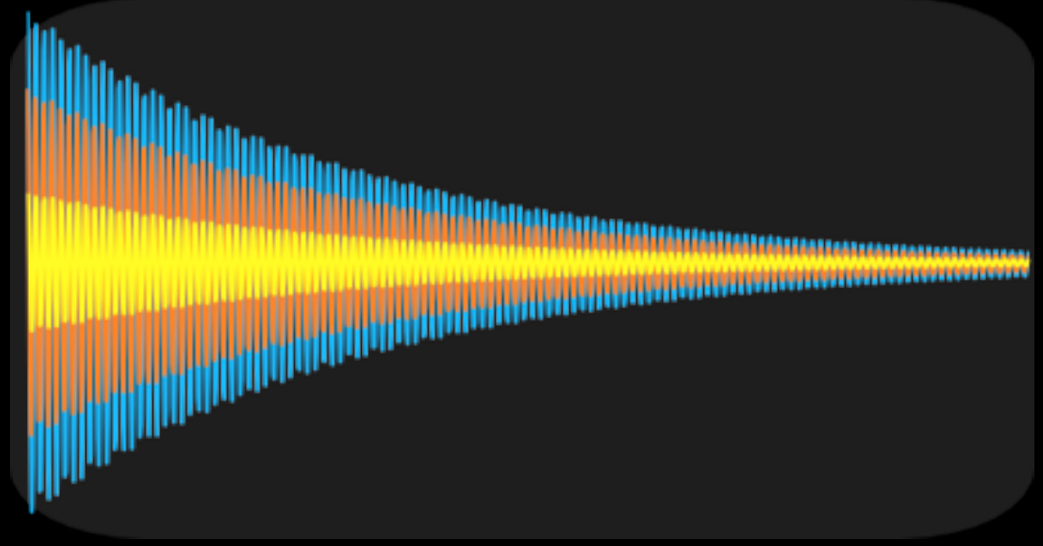

frequency

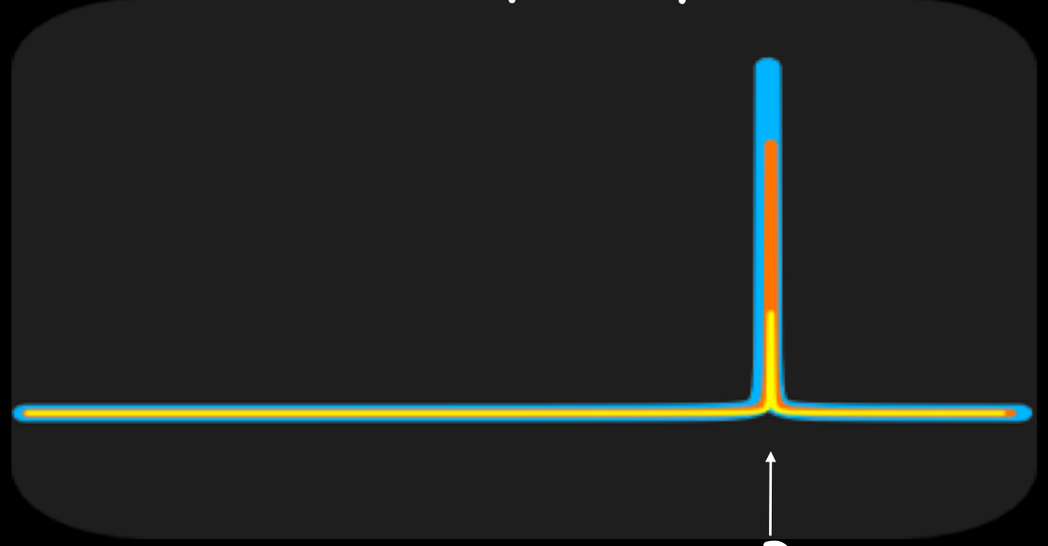

Intro to MRI - Imaging

- B_0 Missing spatial information
- Add gradient field, G

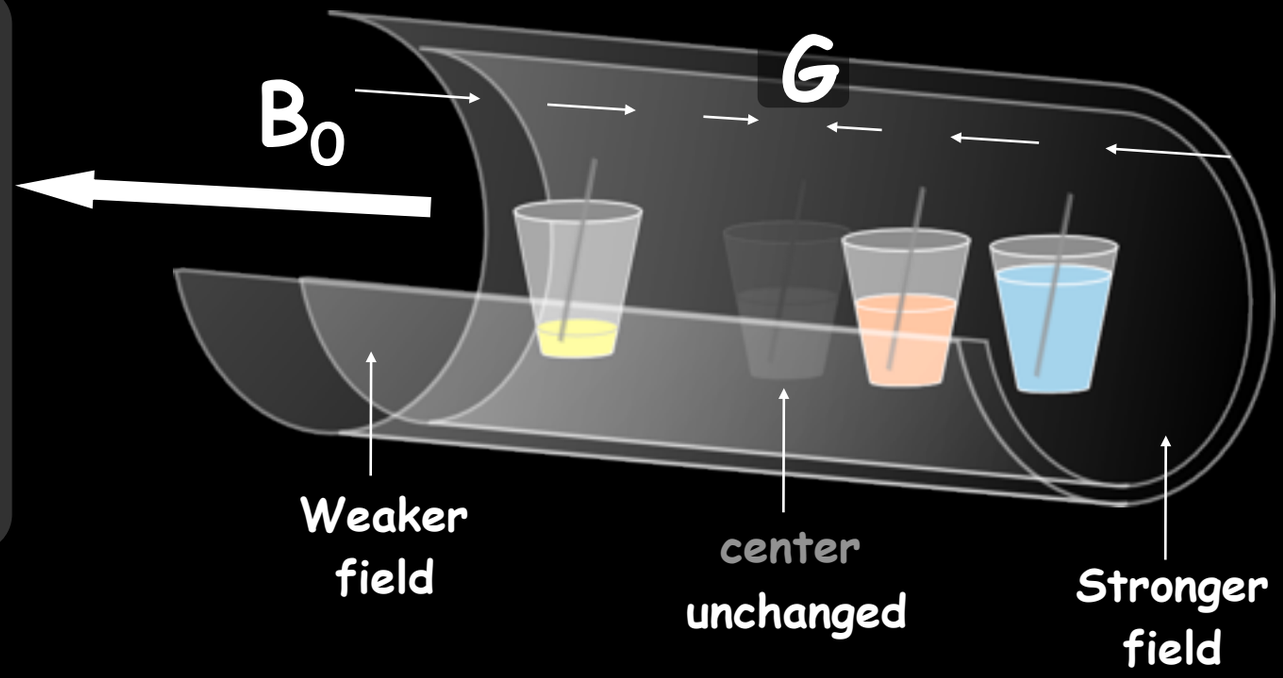

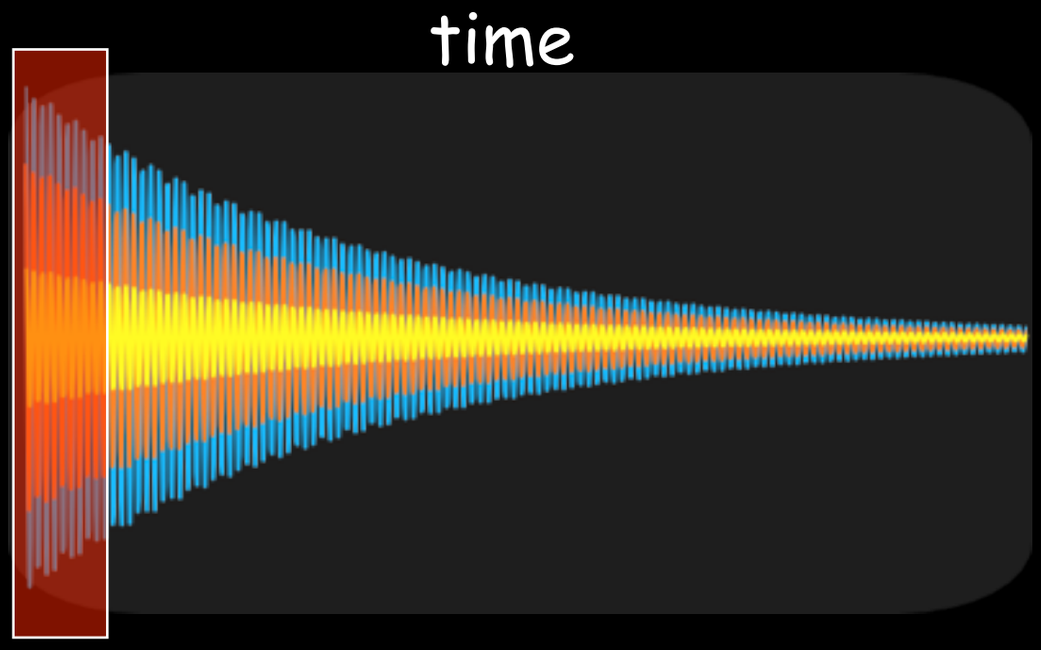

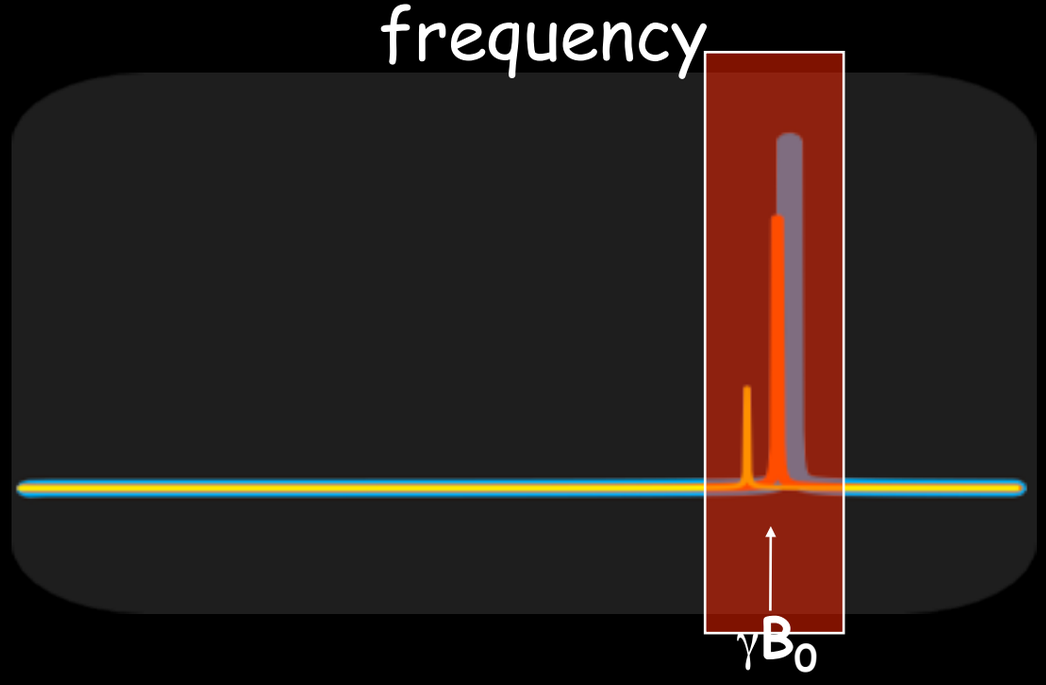

Intro to MRI - Imaging

- B_0 Missing spatial information
- Add gradient field, G
- Mapping:
  spatial position ⇒ frequency

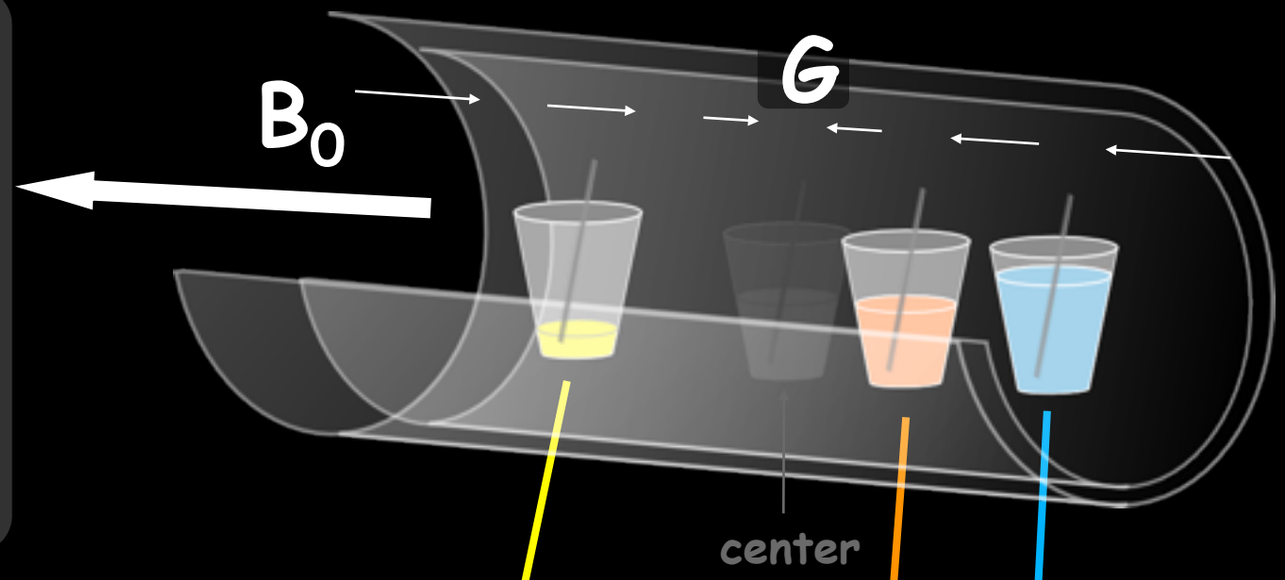

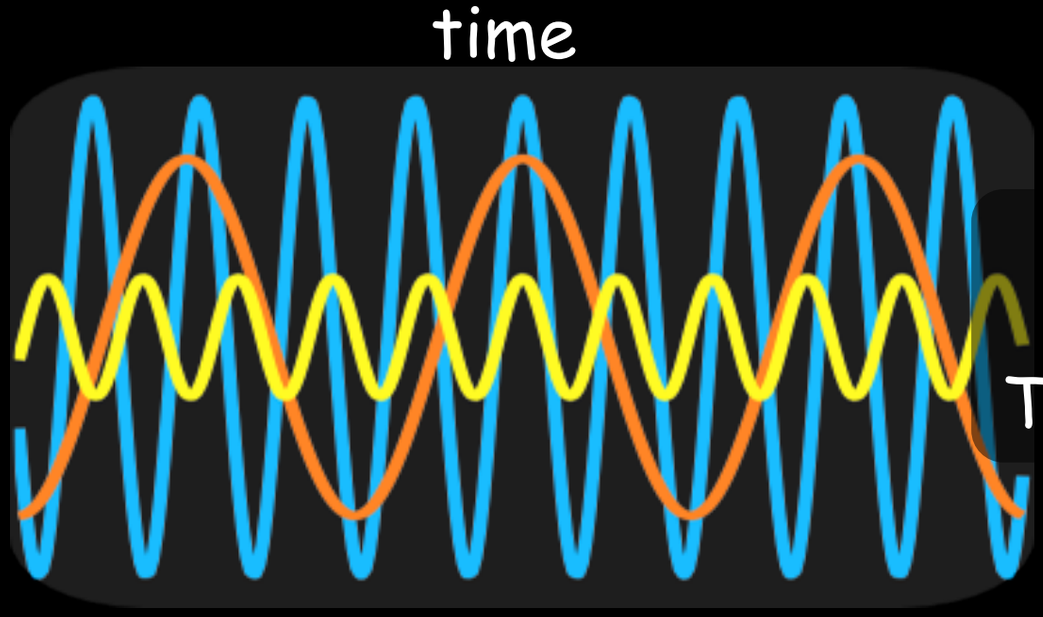

Fourier Transform

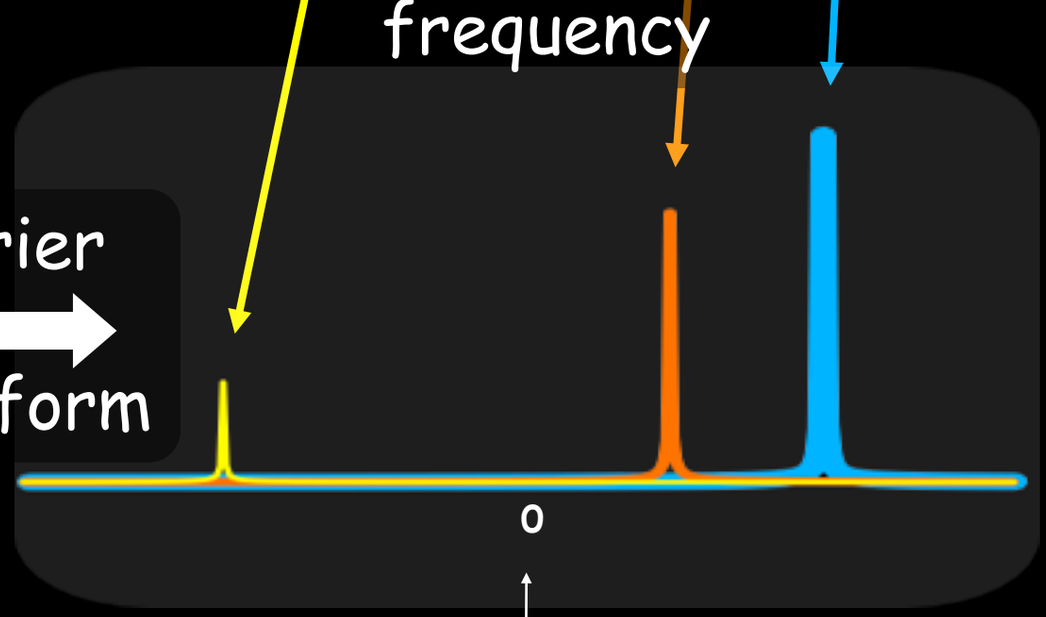

Tuning Fork Demo

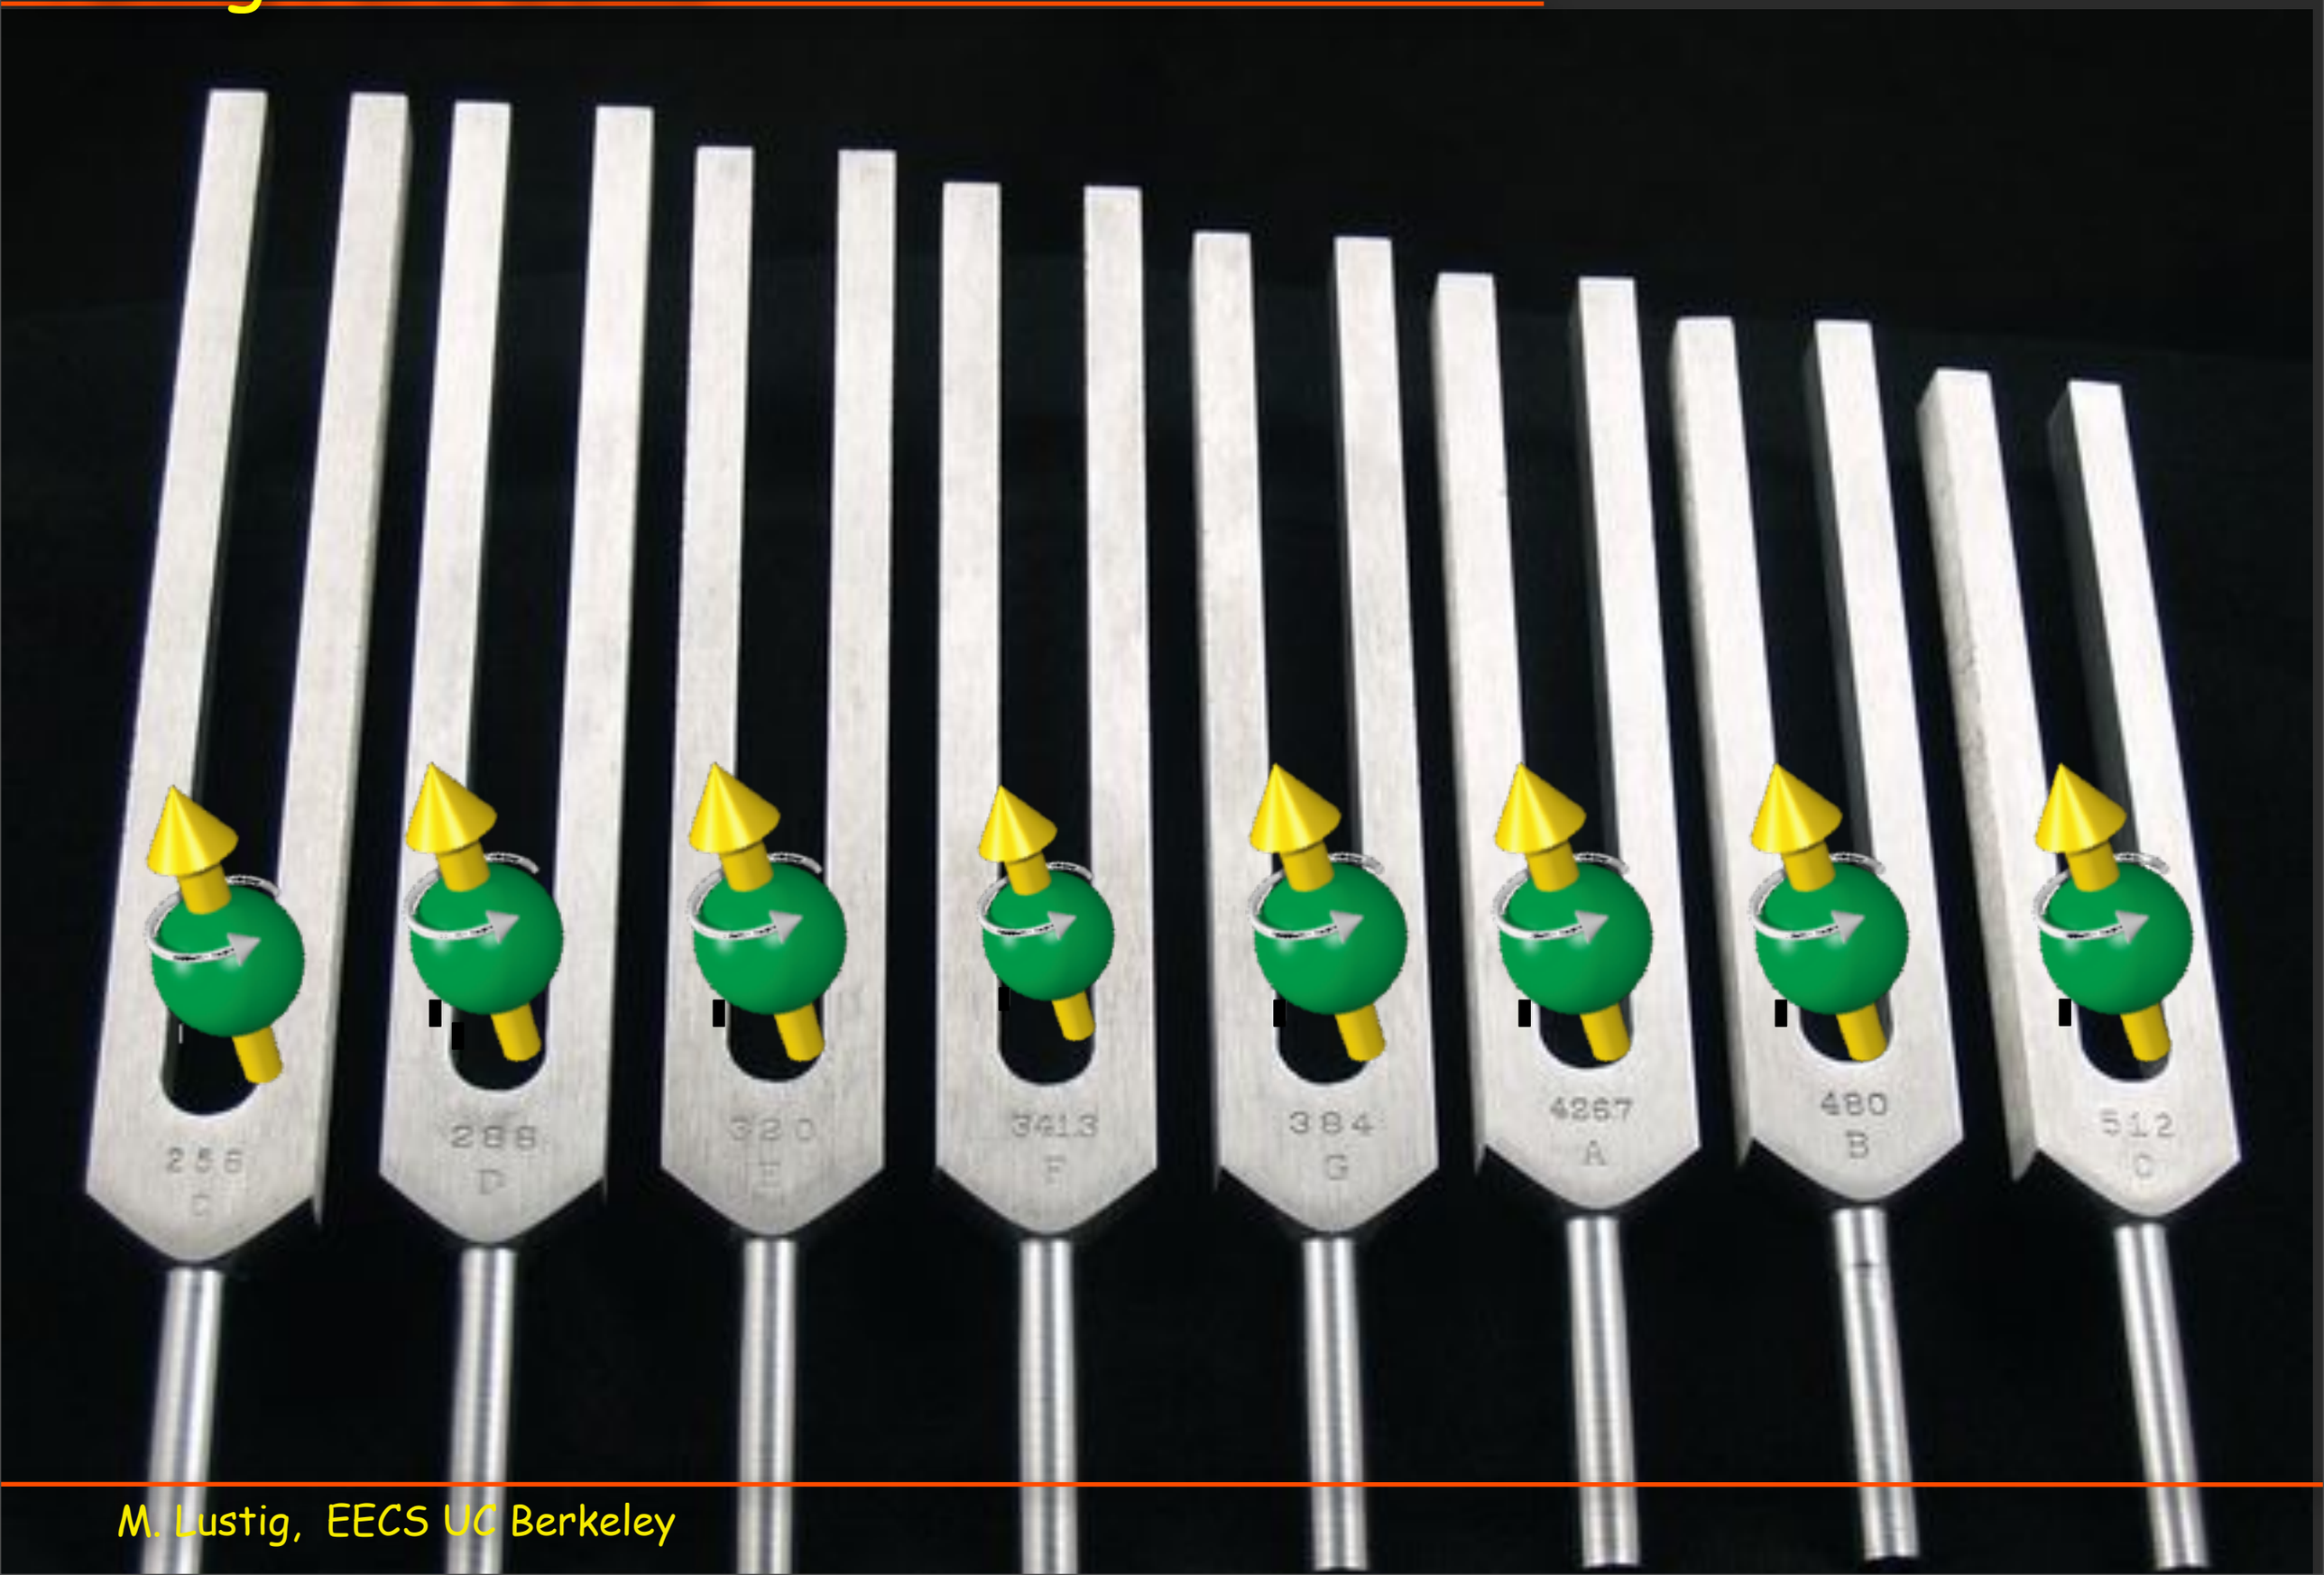

MR Imaging

Fourier

k-space (Raw Data)

Image

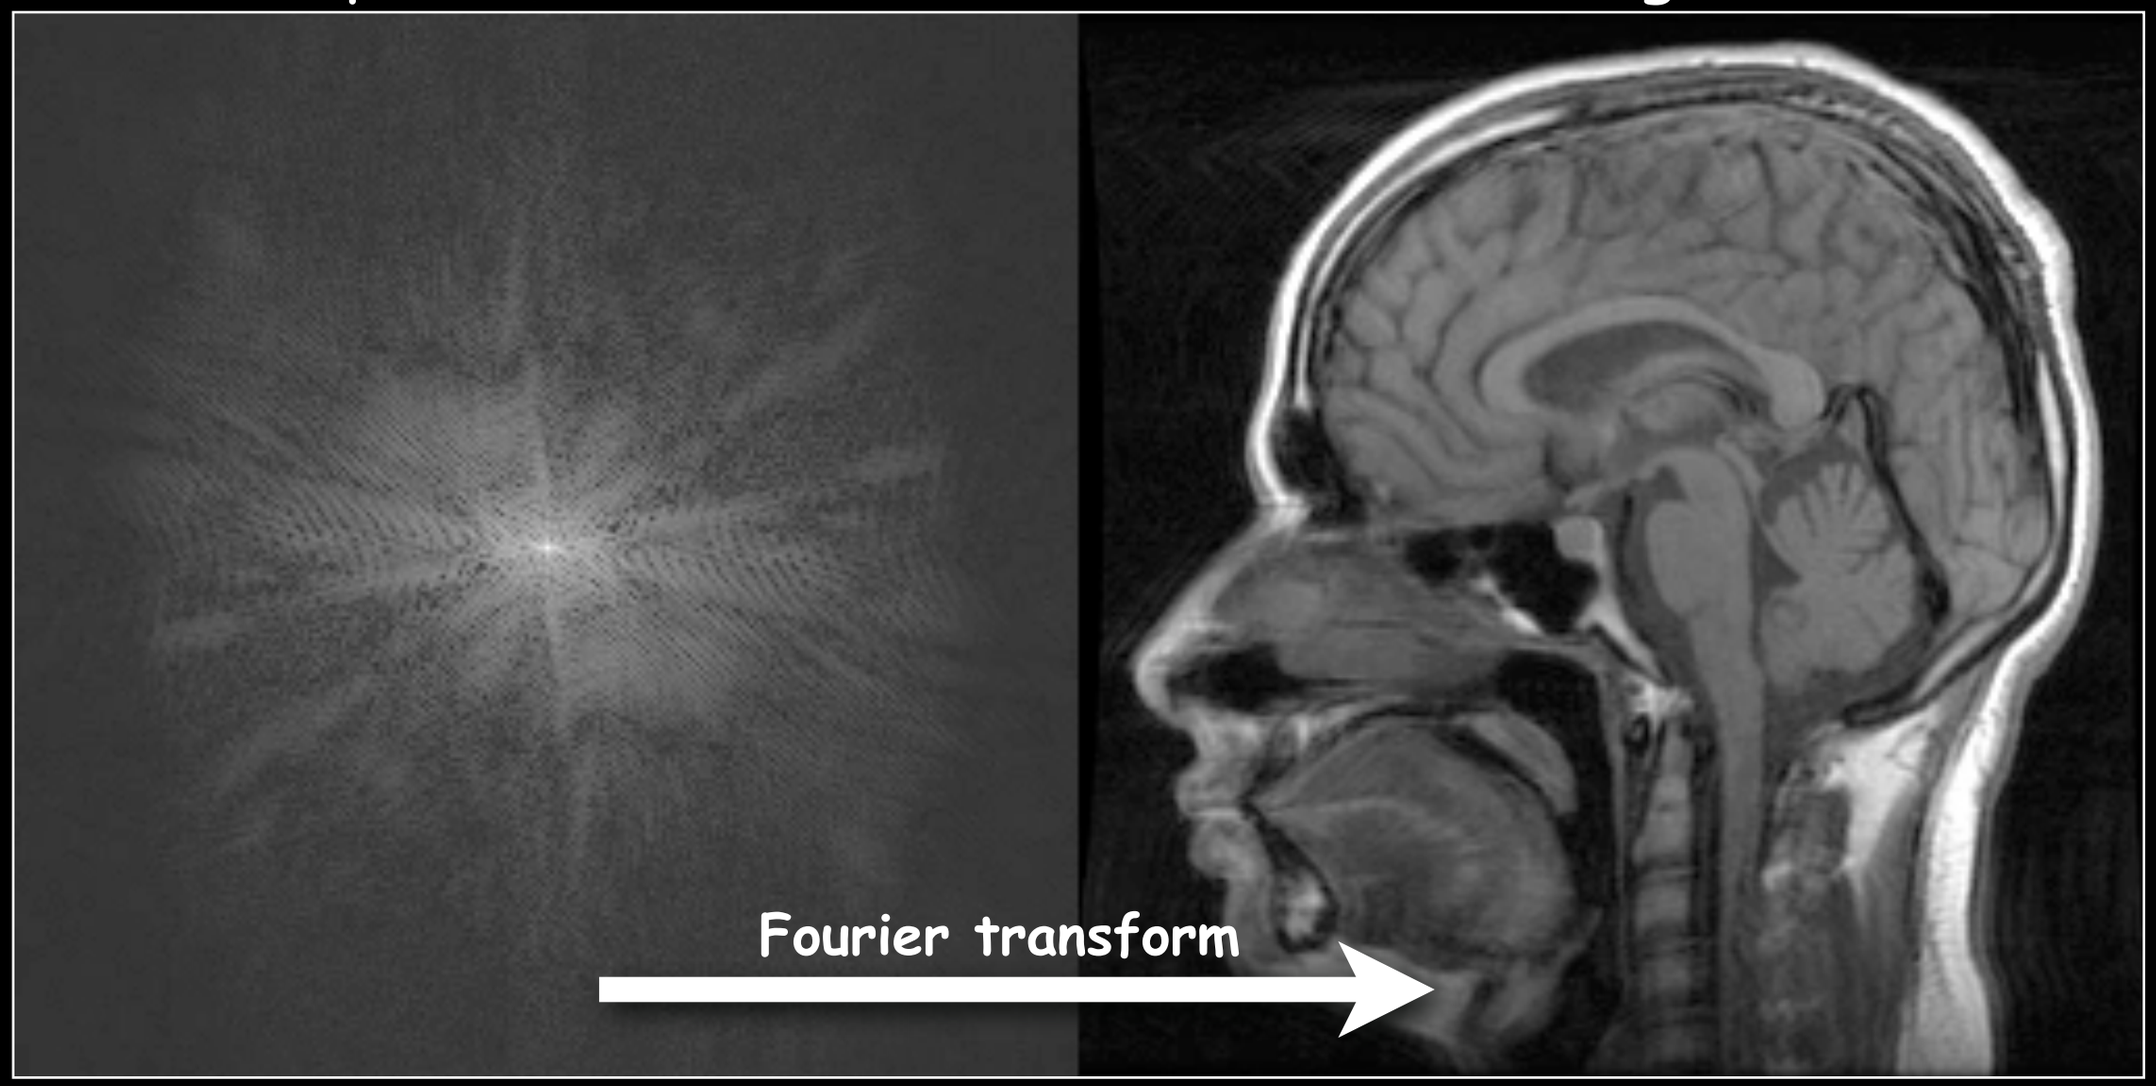

k-space Sampling - resolution

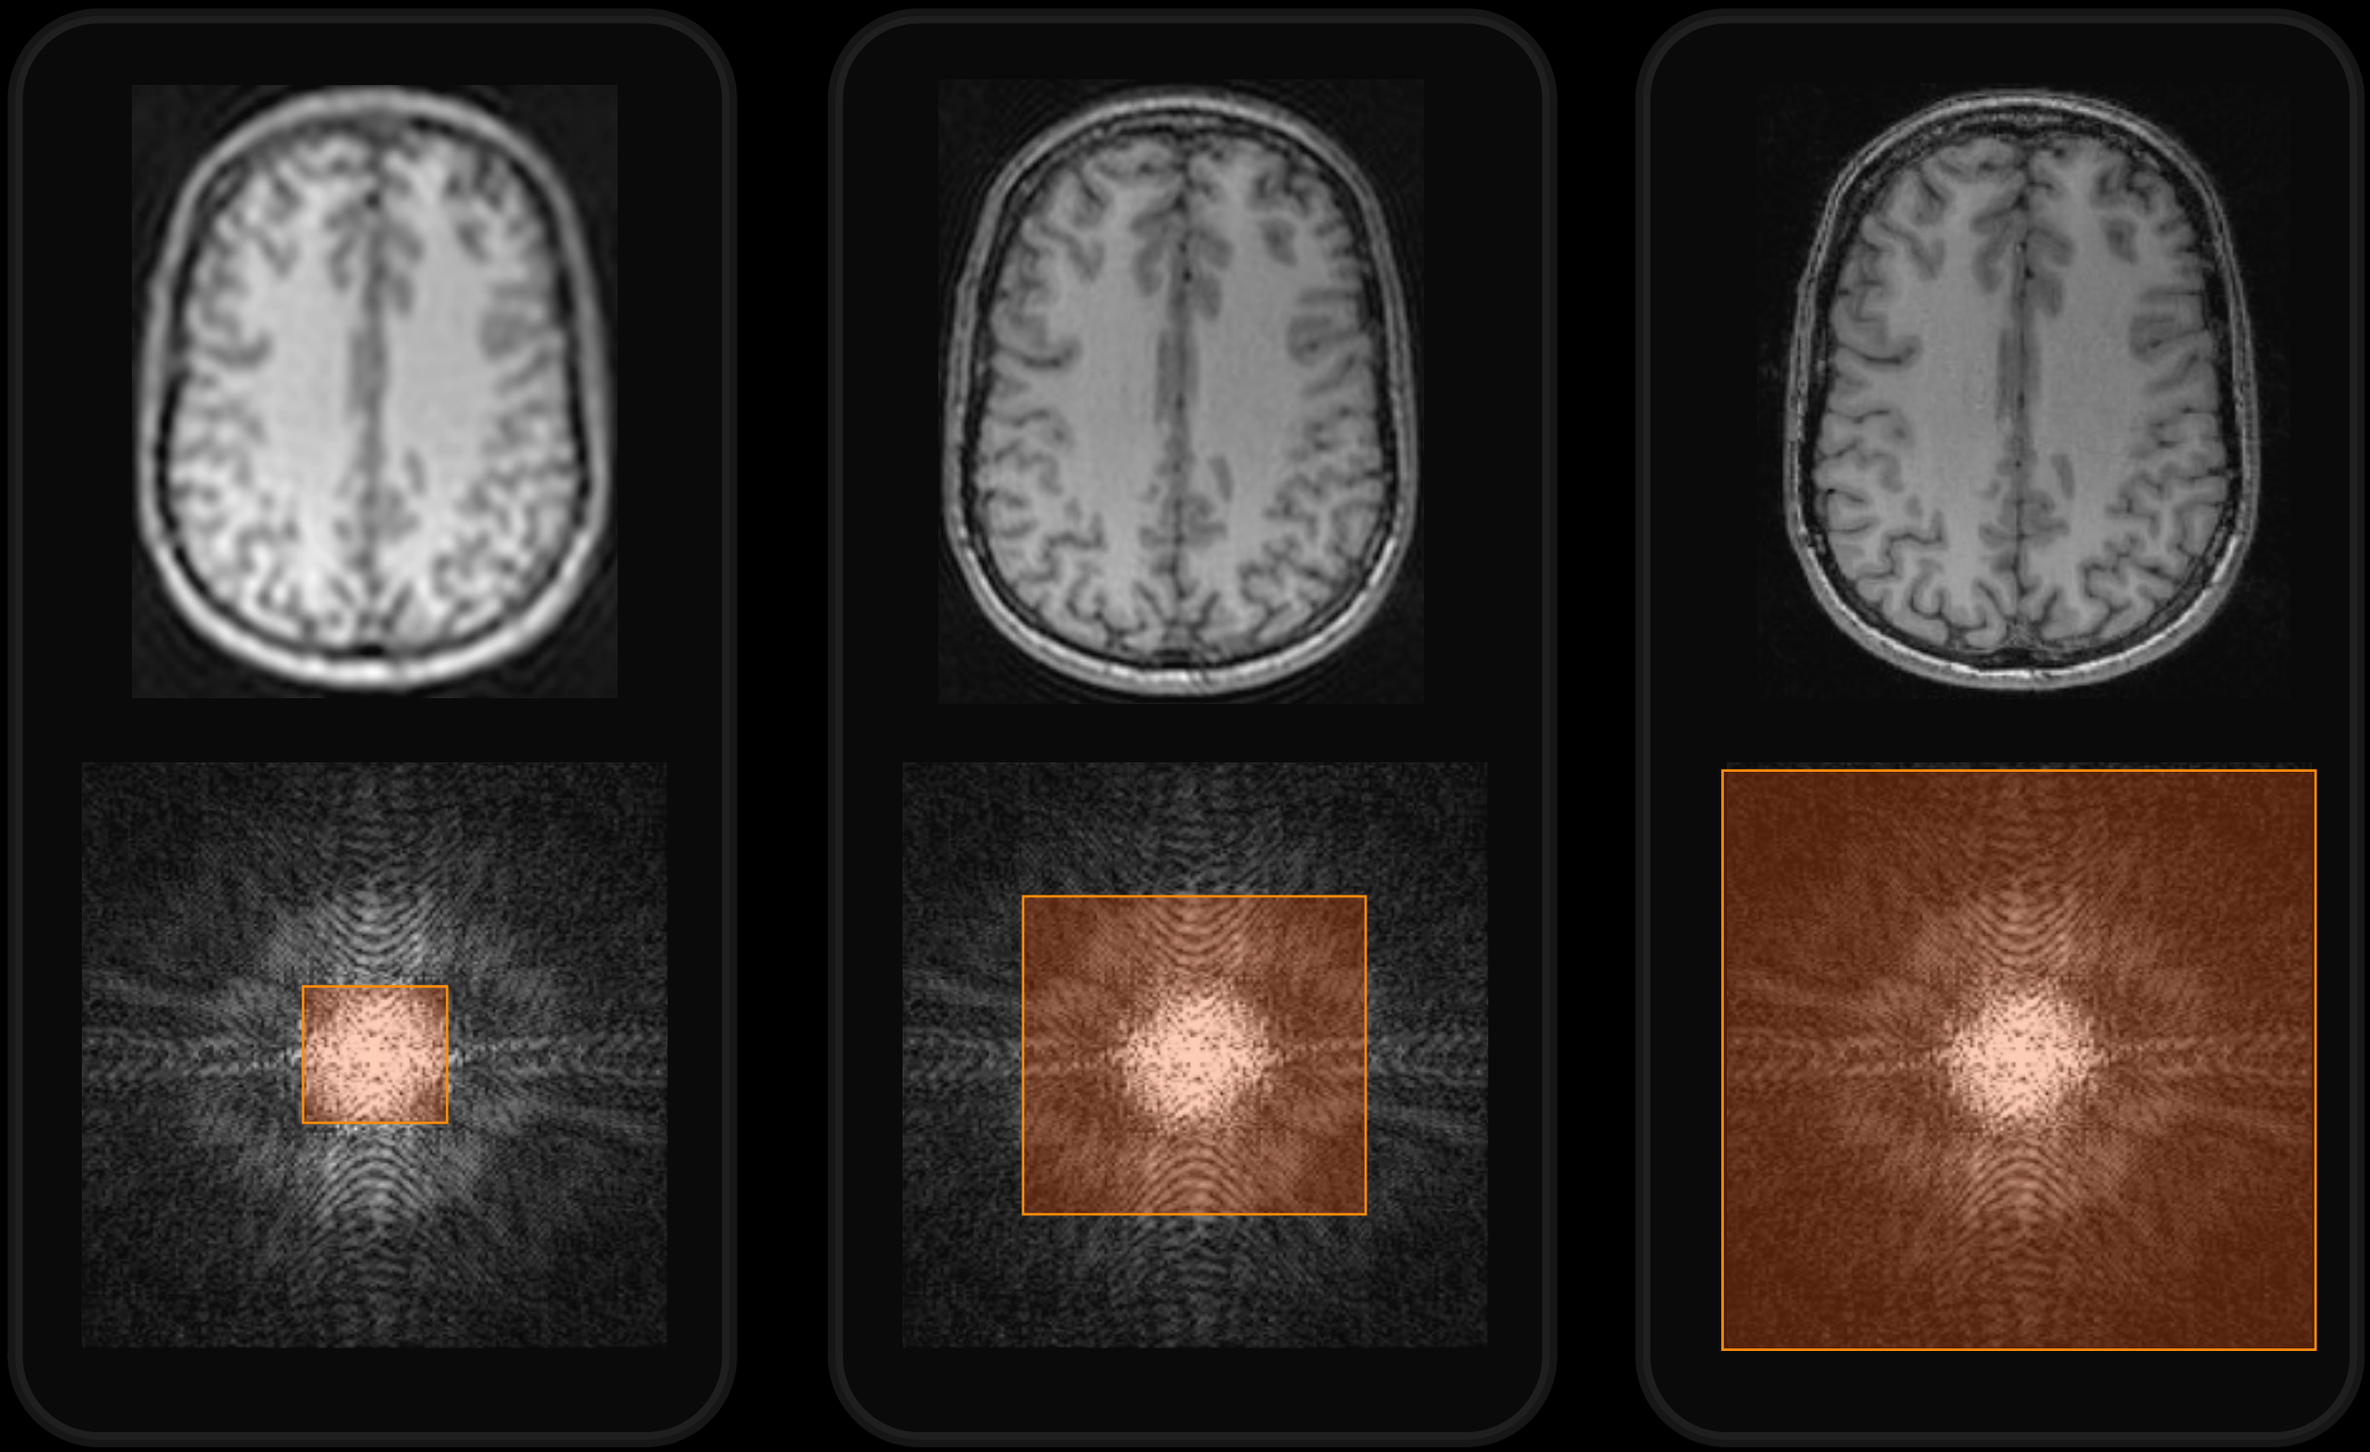

k-space Sampling - FOV

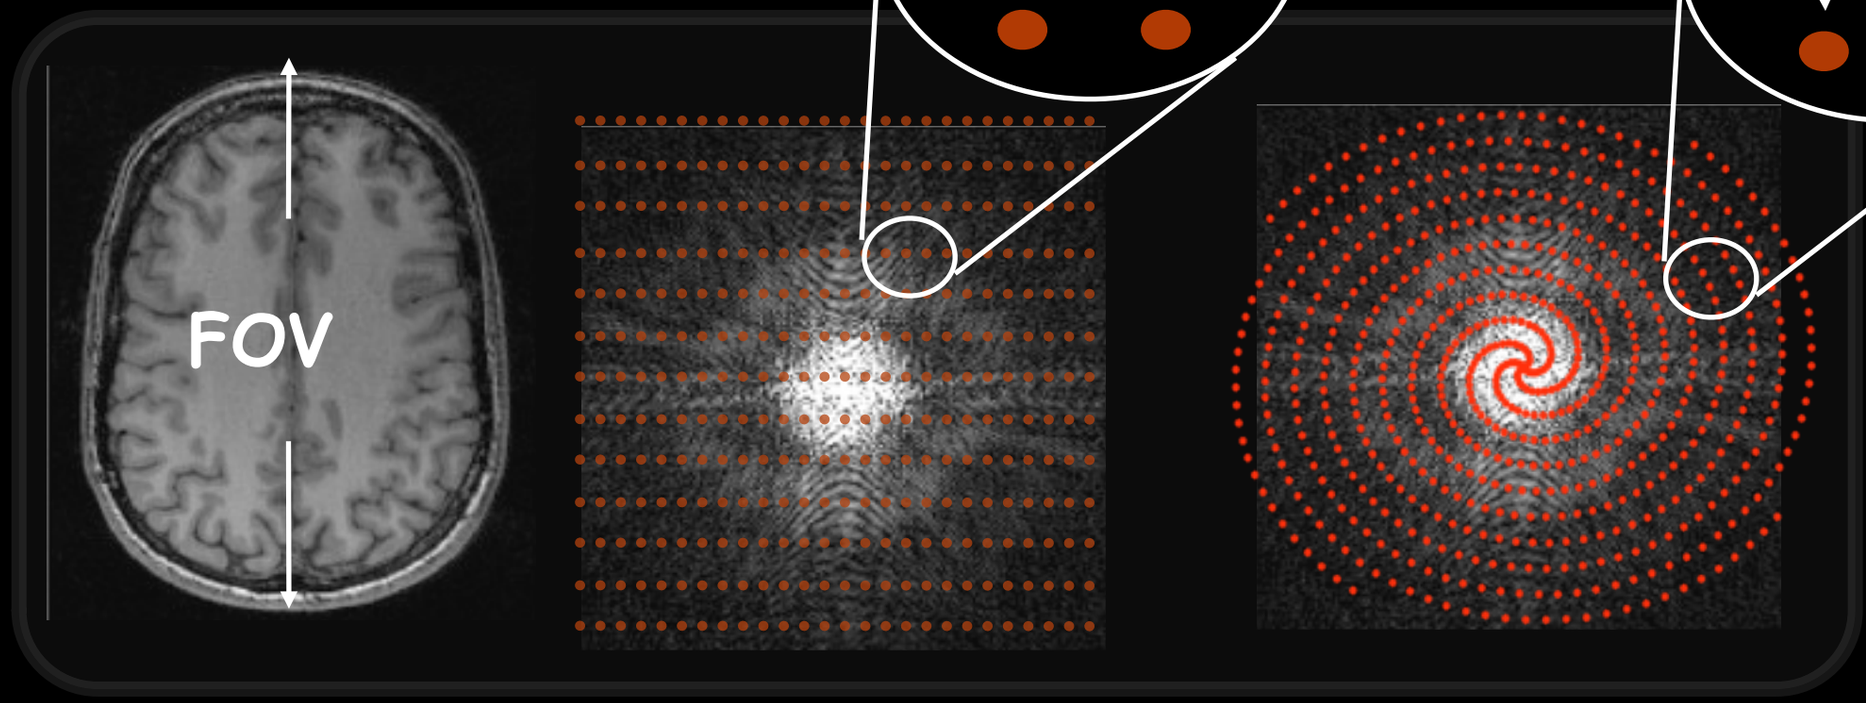

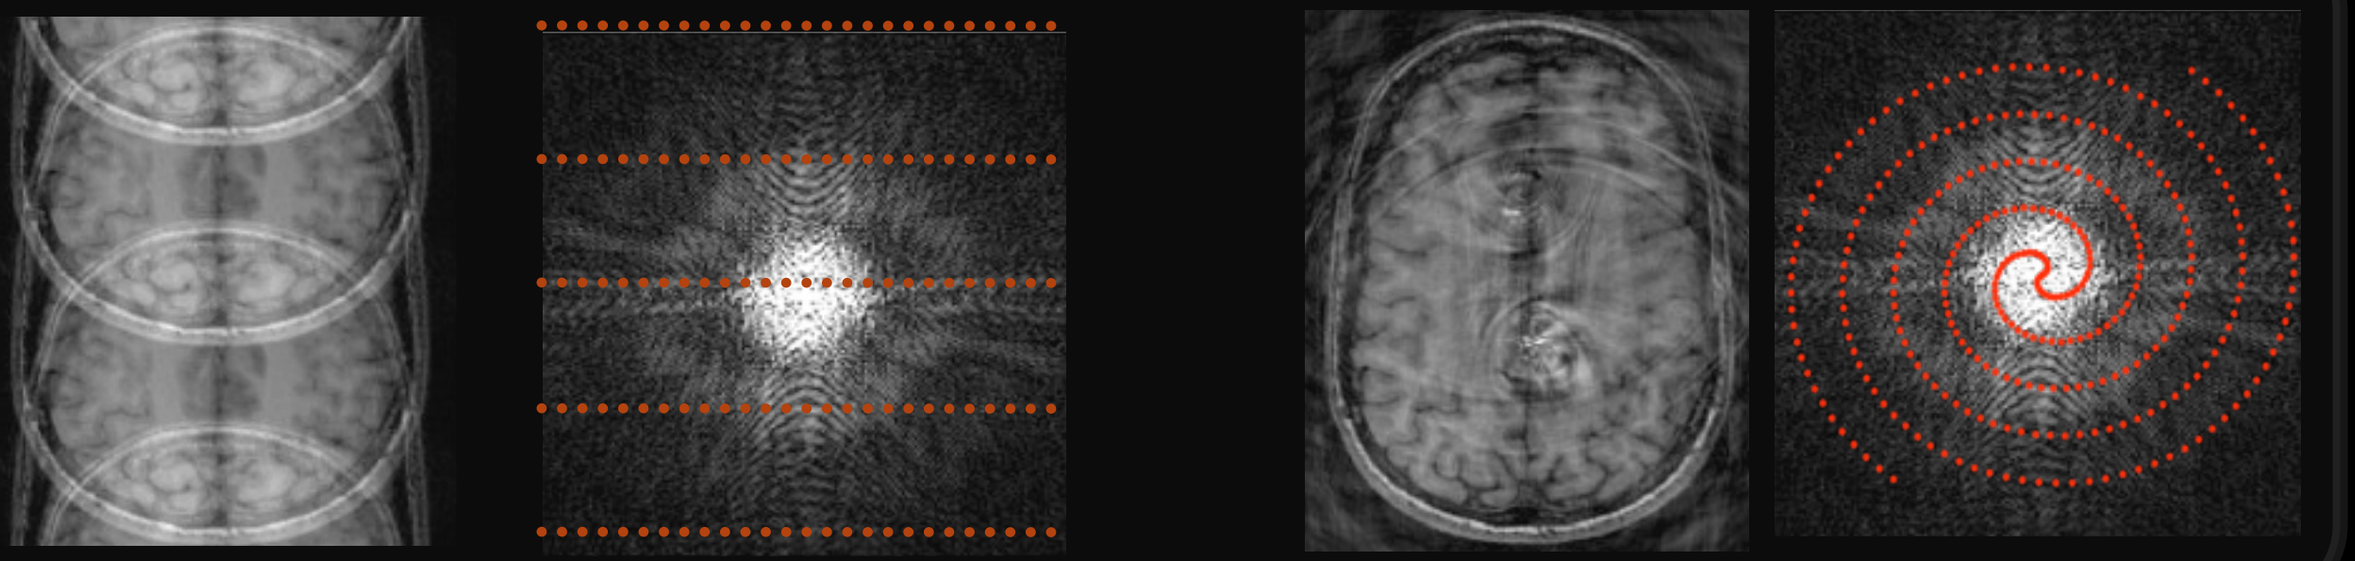

MRI is all about contrast……

Relaxation

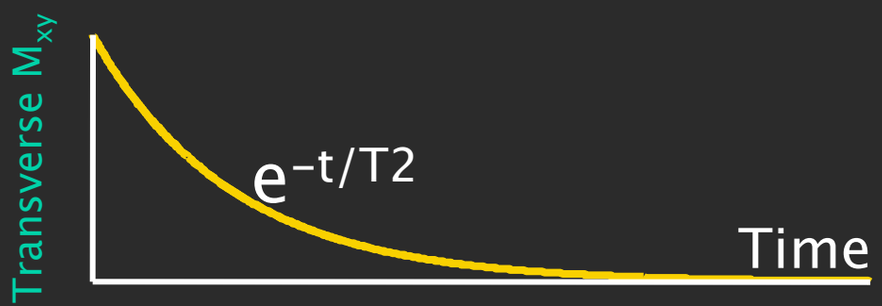

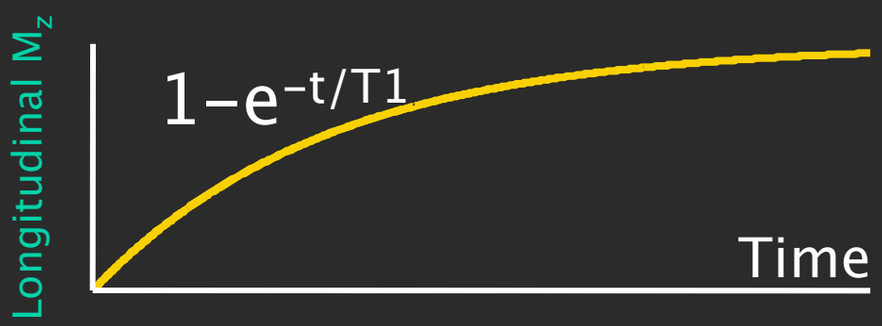

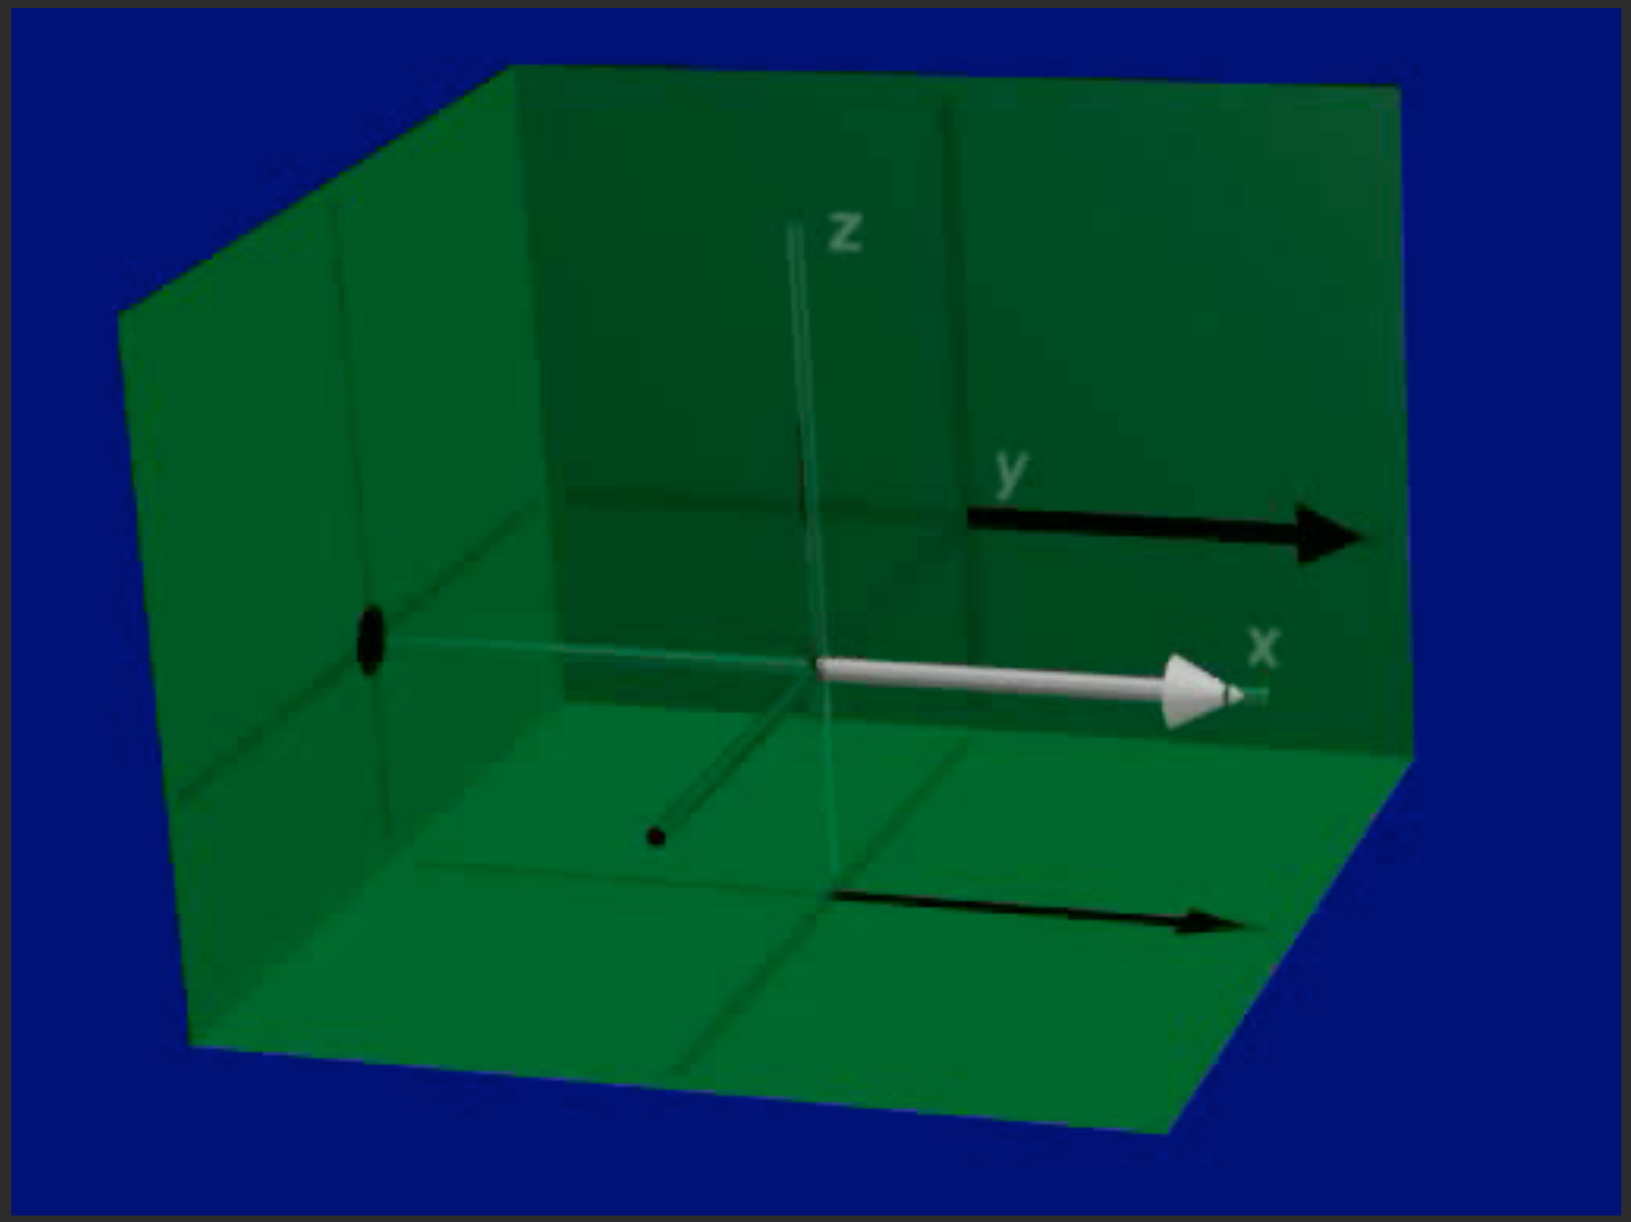

The Toilette Analogy (©2009 Al Macovski)

- Excitation = Flush

- T2 = Active flushing ~5 second

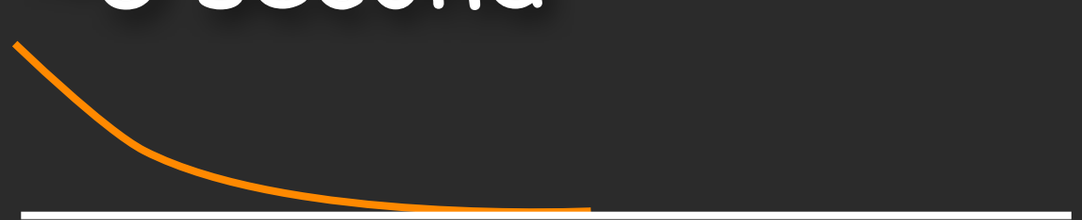

- T1 = Refilling time ~1min

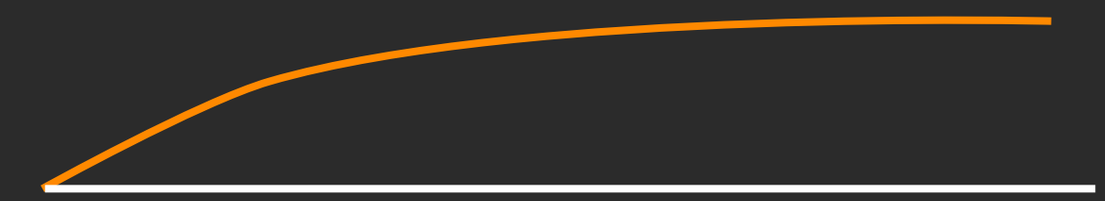

The Toilette Analogy, Steady-state

- Flush - Refill

- Flush continuously
  - Never fully refills
  - After a while, same from flush to flush
  - "Steady state"
- Timing creates contrast

Contrast

T1

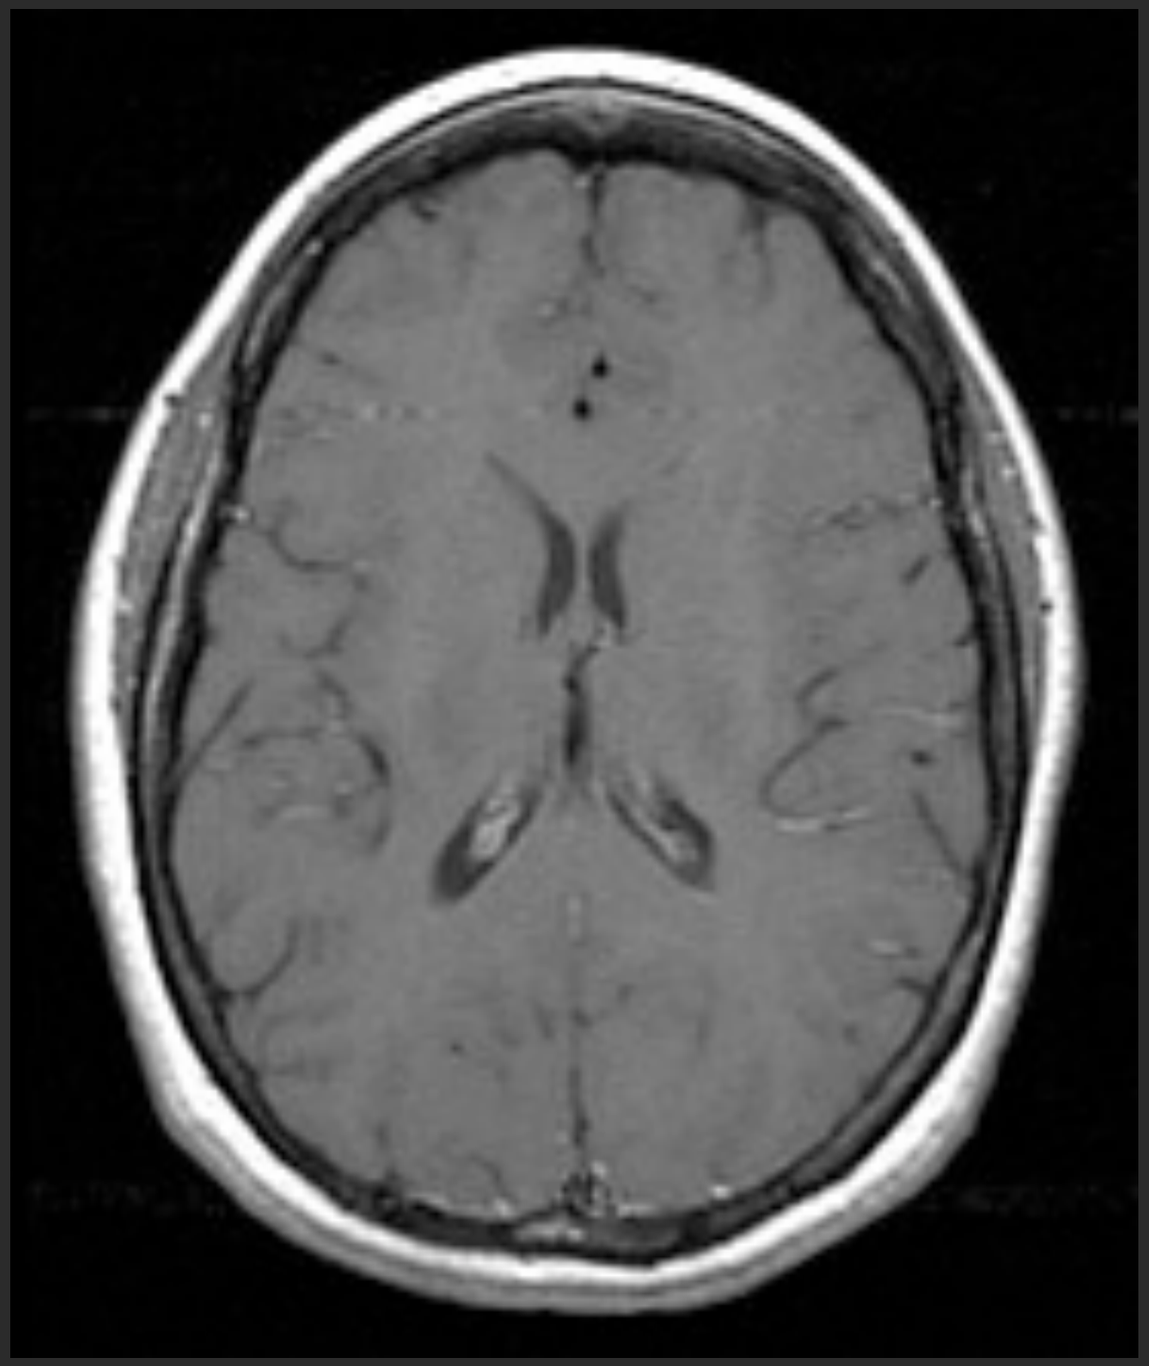

T2

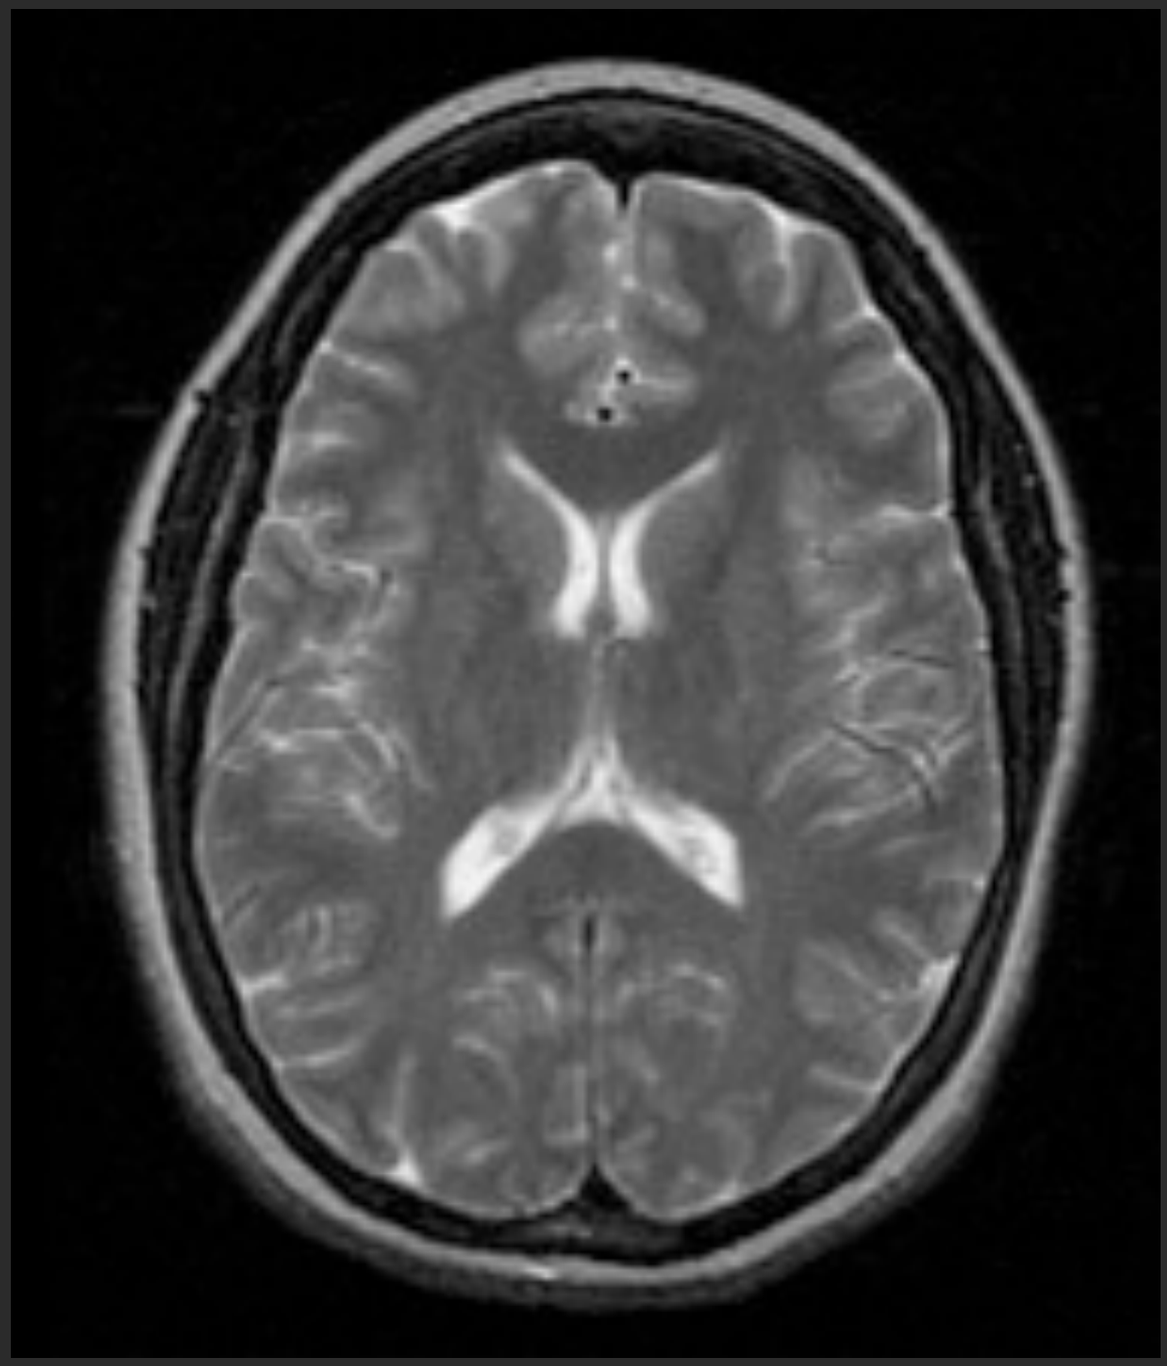

House Prefers T2 .....

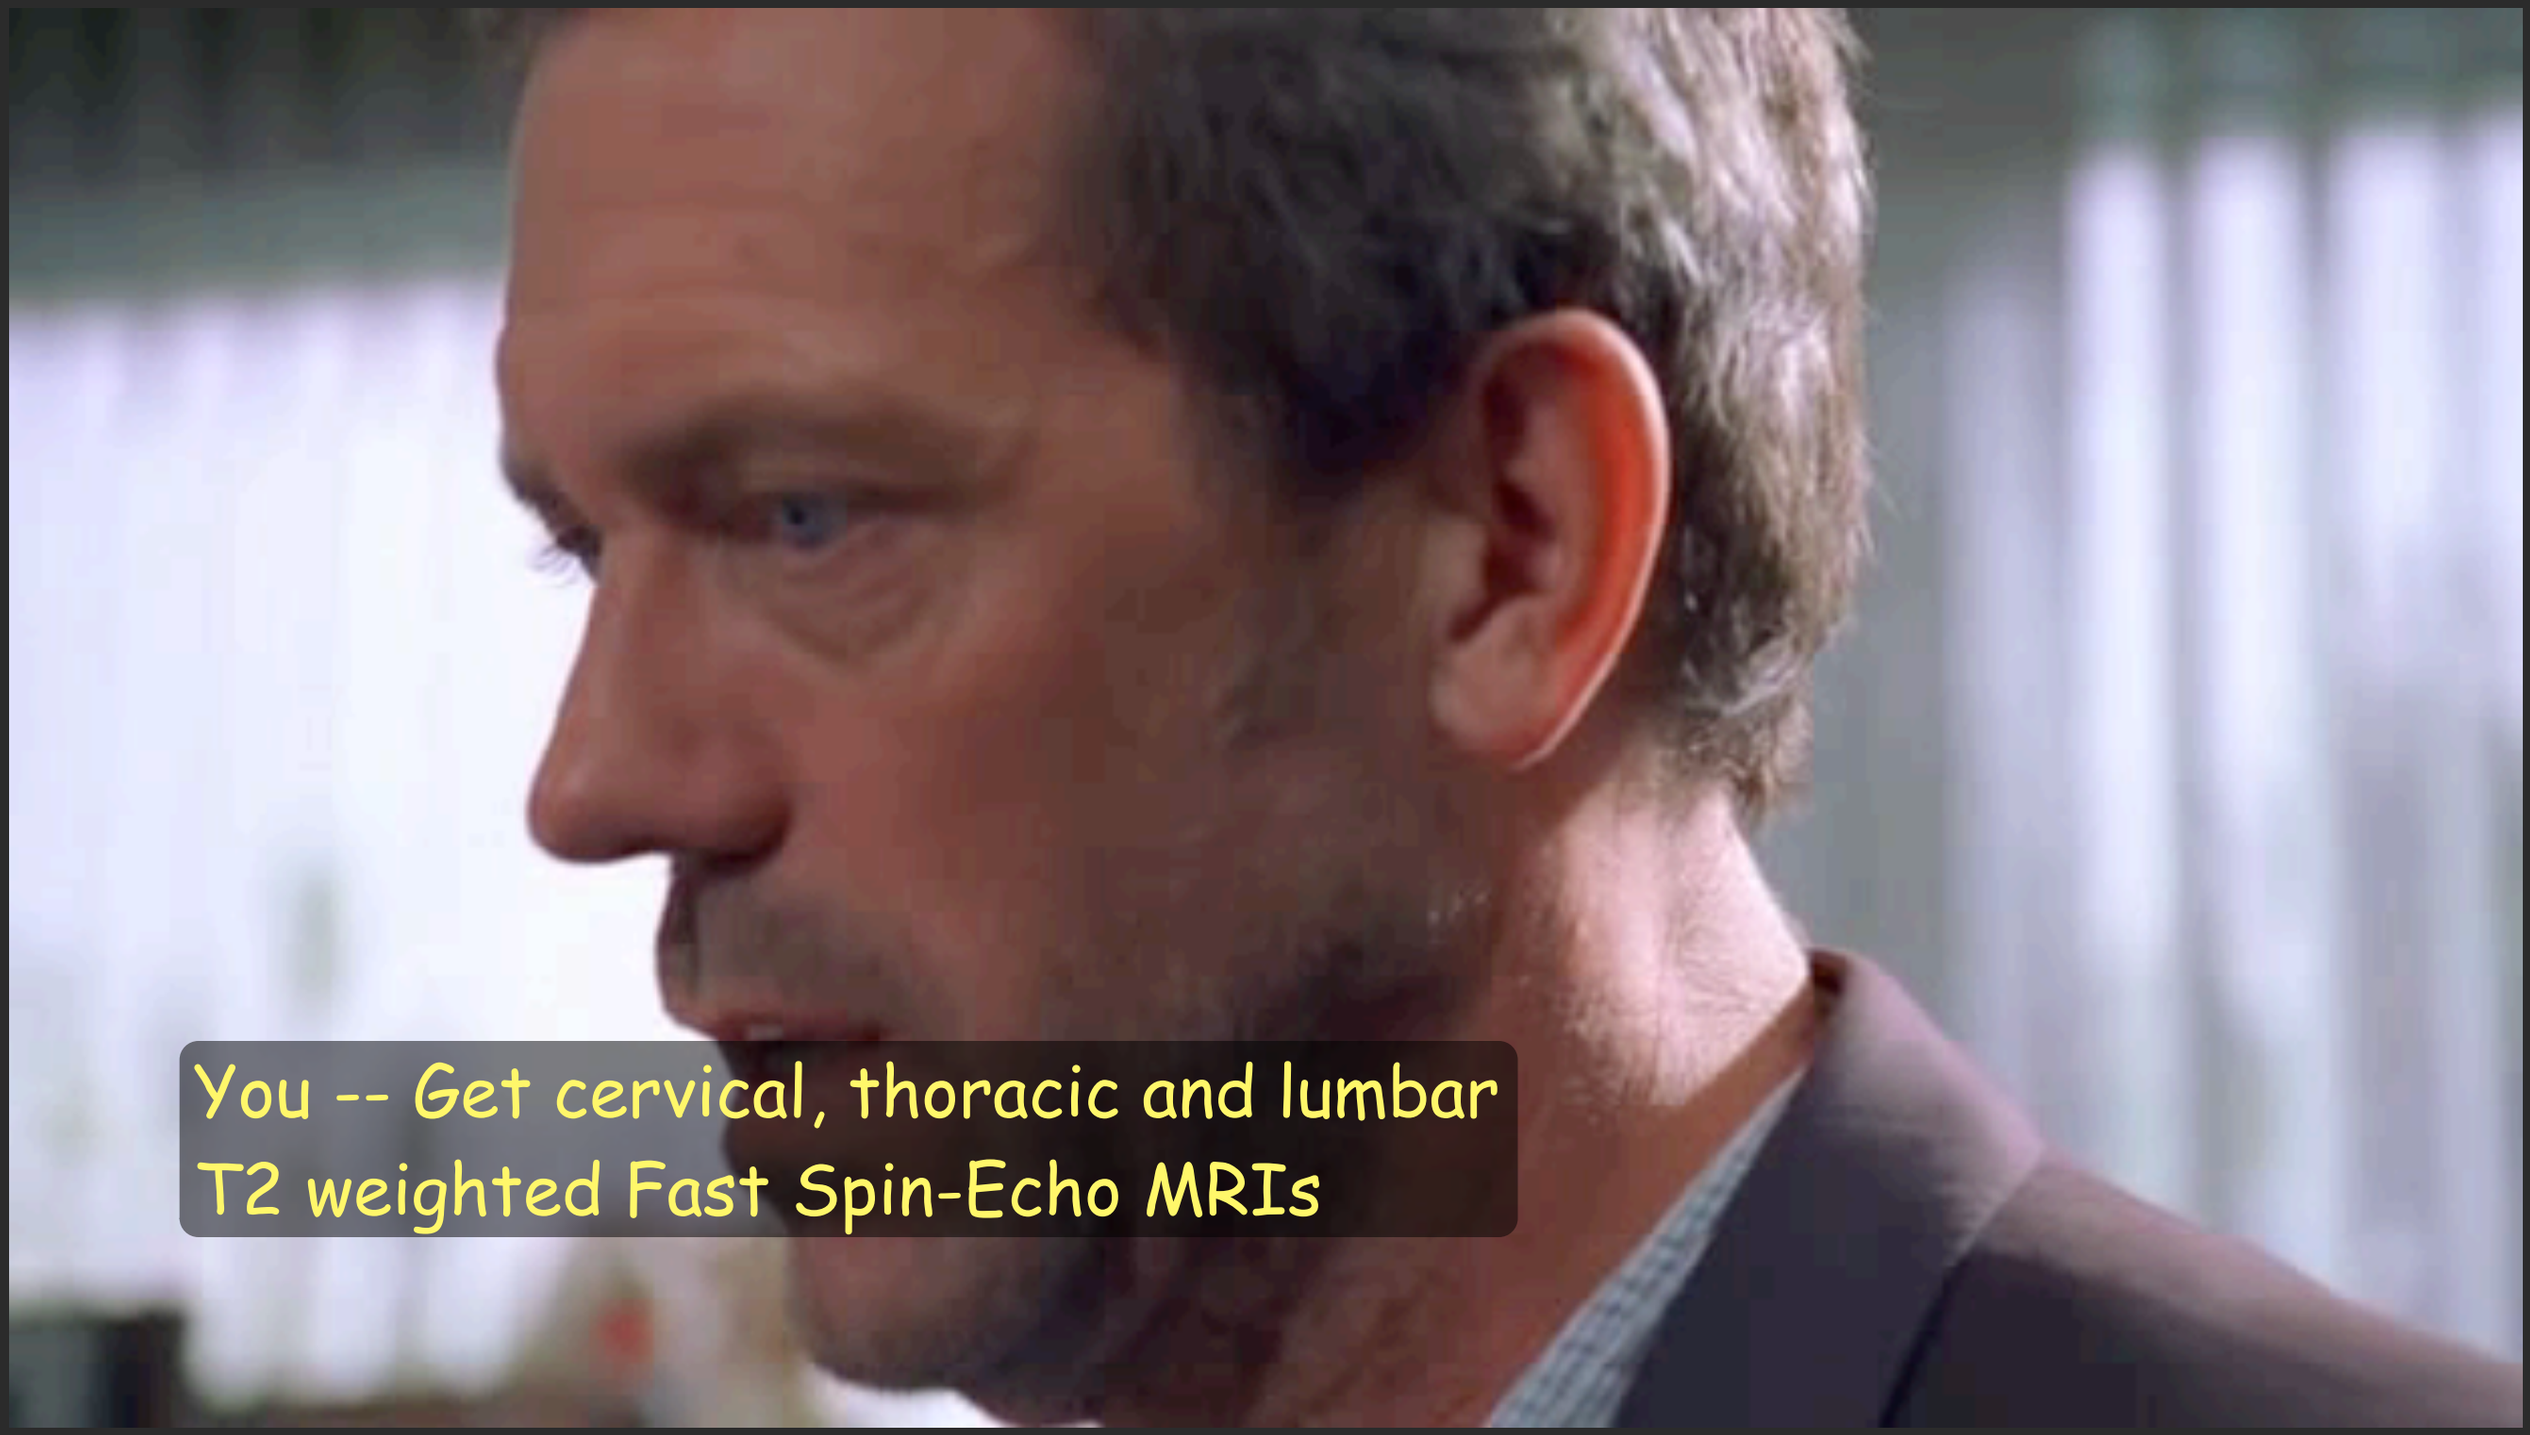

Thank You

תודה רבה

http://www.eecs.berkeley.edu/~mlustig